

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032724\
 Data File : VV034870.D
 Acq On : 27 Mar 2024 17:17
 Operator : SY/MD
 Sample : PB159796TB 10 X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 28 01:57:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 01:53:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	332388	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	331604	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	152162	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	97653	30.421	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	60.840%		
7) Chloroethane-d5	1.529	69	96929	34.765	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	69.520%#		
11) 1,1-Dichloroethene-d2	2.057	65	47104	33.475	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.960%		
21) 2-Butanone-d5	3.783	46	162587	85.401	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	85.400%		
24) Chloroform-d	4.246	84	216700	40.151	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.300%		
26) 1,2-Dichloroethane-d4	4.941	65	140755	41.077	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.160%		
32) Benzene-d6	4.960	84	405535	36.408	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	72.820%		
36) 1,2-Dichloropropane-d6	5.989	67	139743	39.508	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	79.020%		
41) Toluene-d8	7.243	98	347563	34.648	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	69.300%#		
43) trans-1,3-Dichloroprop...	7.551	79	61067	35.514	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.020%		
47) 2-Hexanone-d5	8.021	63	113127	84.593	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	84.590%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	211344	43.390	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.780%		
66) 1,2-Dichlorobenzene-d4	11.558	152	146177	42.787	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.580%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	9482	5.425	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032724\
Data File : VV034870.D
Acq On : 27 Mar 2024 17:17
Operator : SY/MD
Sample : PB159796TB 10 X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 28 01:57:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 01:53:40 2024
Response via : Initial Calibration

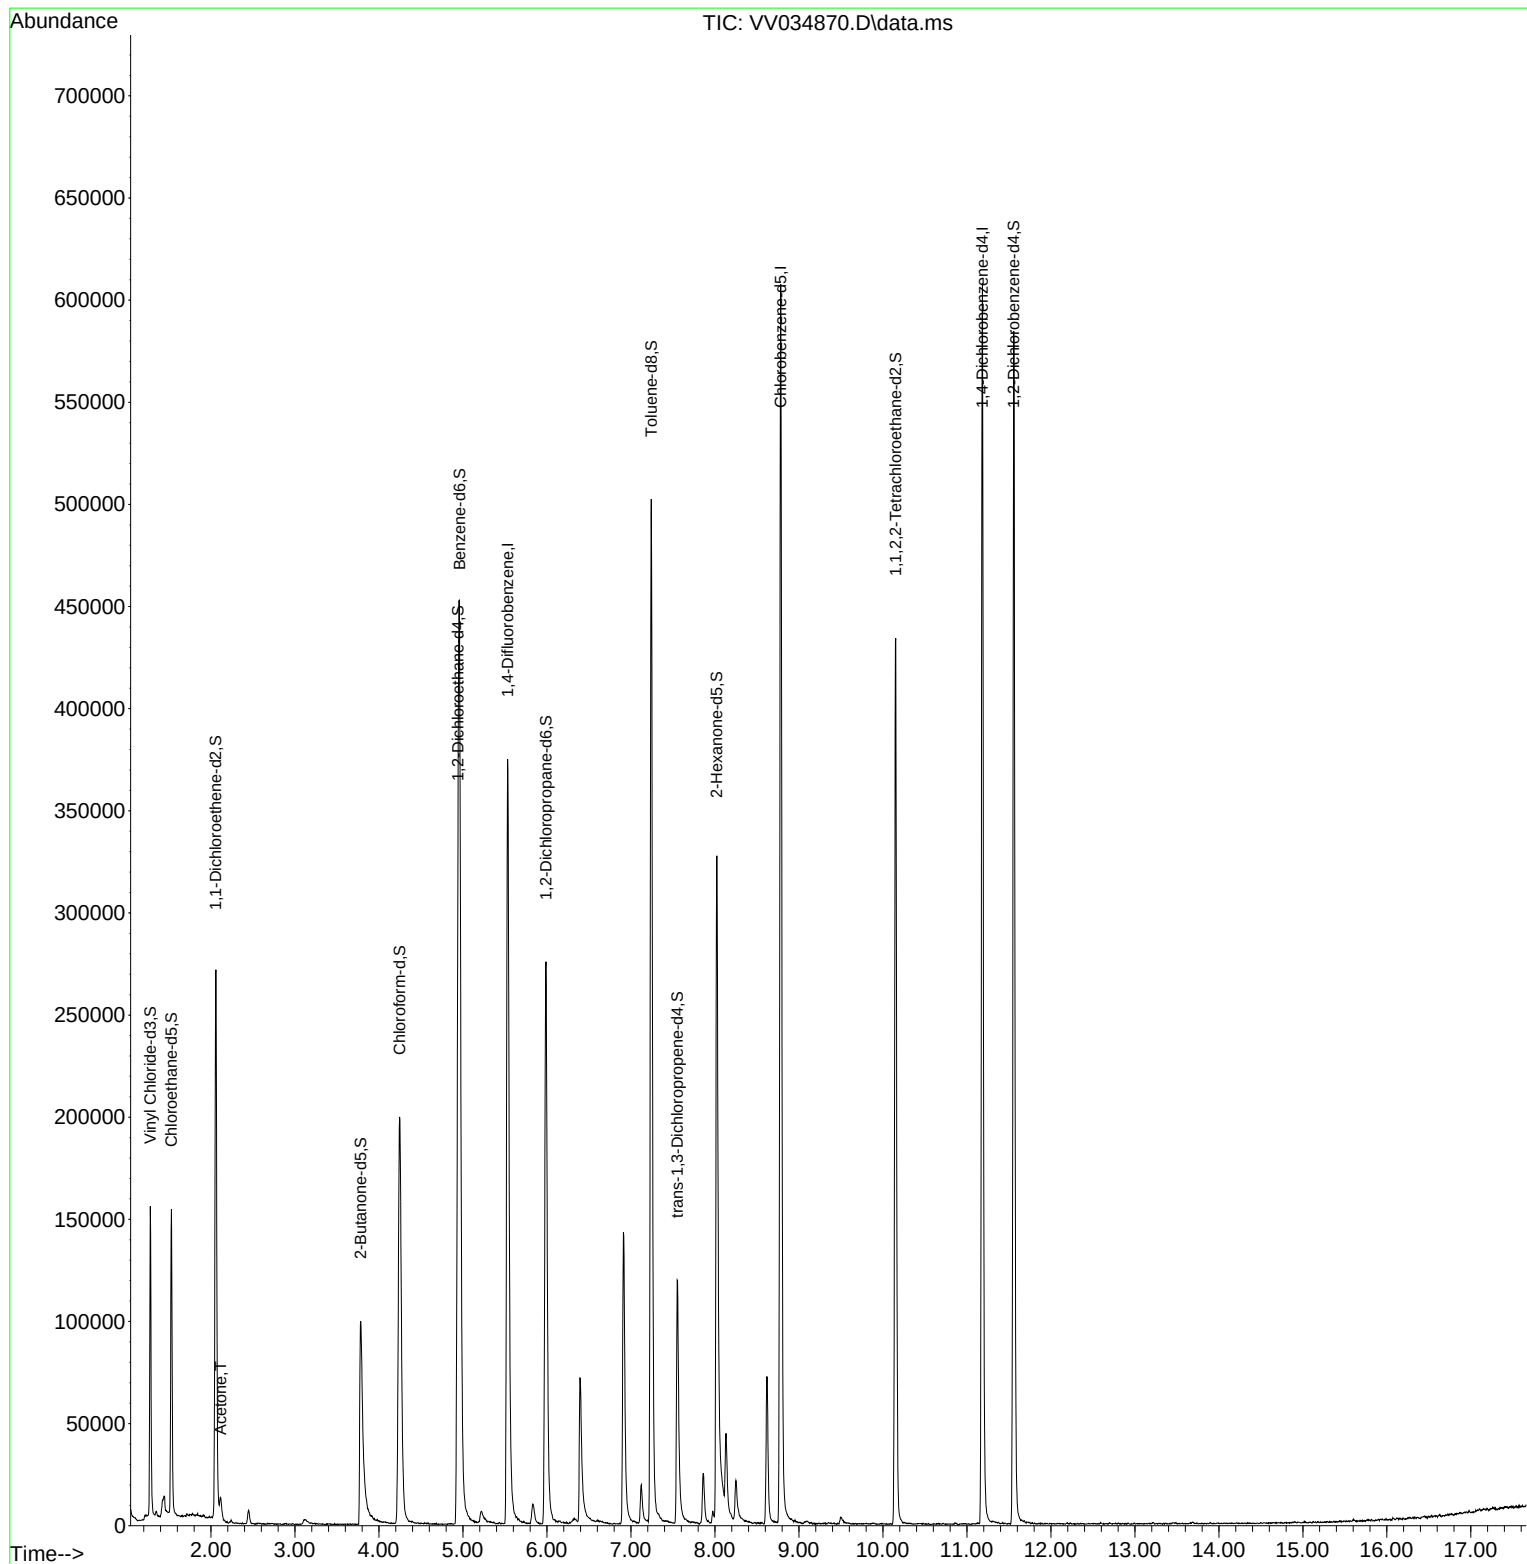

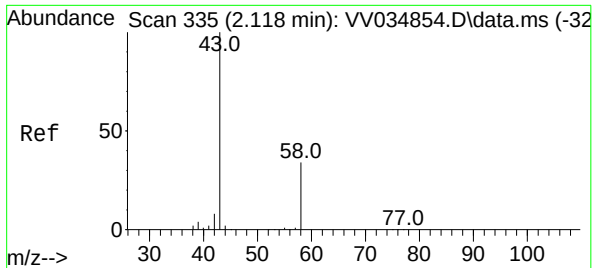

#13

Acetone

Concen: 5.425 ug/L

RT: 2.114 min Scan# 34

Delta R.T. -0.003 min


Lab File: VV034870.D

Acq: 27 Mar 2024 17:17

Instrument :

MSVOA_V

ClientSampleId :

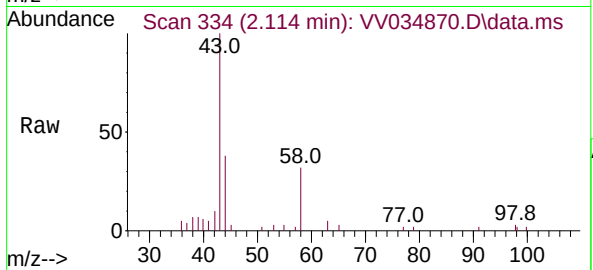

Tgt Ion: 43 Resp: 9482

Ion Ratio Lower Upper

43 100

58 29.1 0.0 66.0

