




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025250.D
Acq On : 28 Mar 2022 10:44
Operator : SY/MD
Sample : VV0328wBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/29/2022
Supervised By :Mahesh Dadoda 04/01/2022

Quant Time: Mar 29 03:40:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

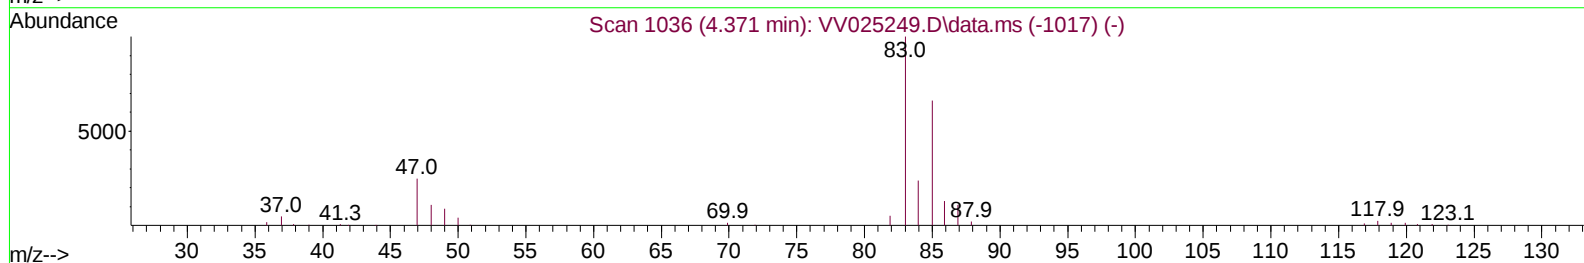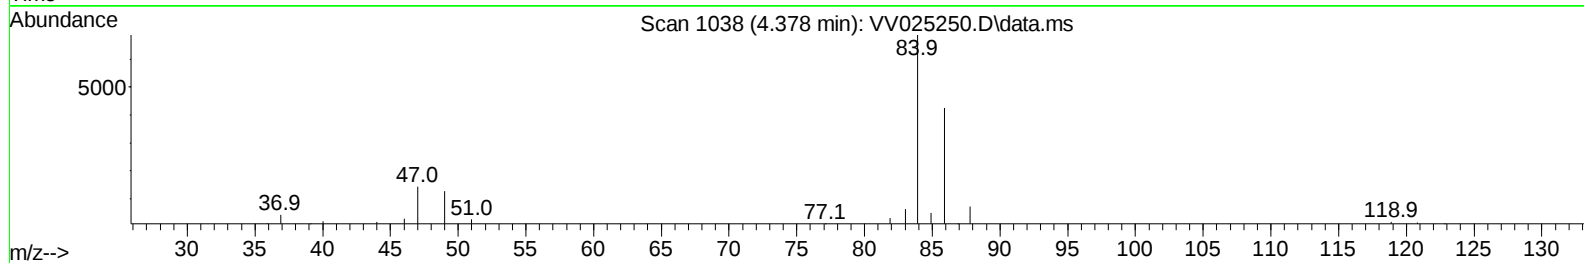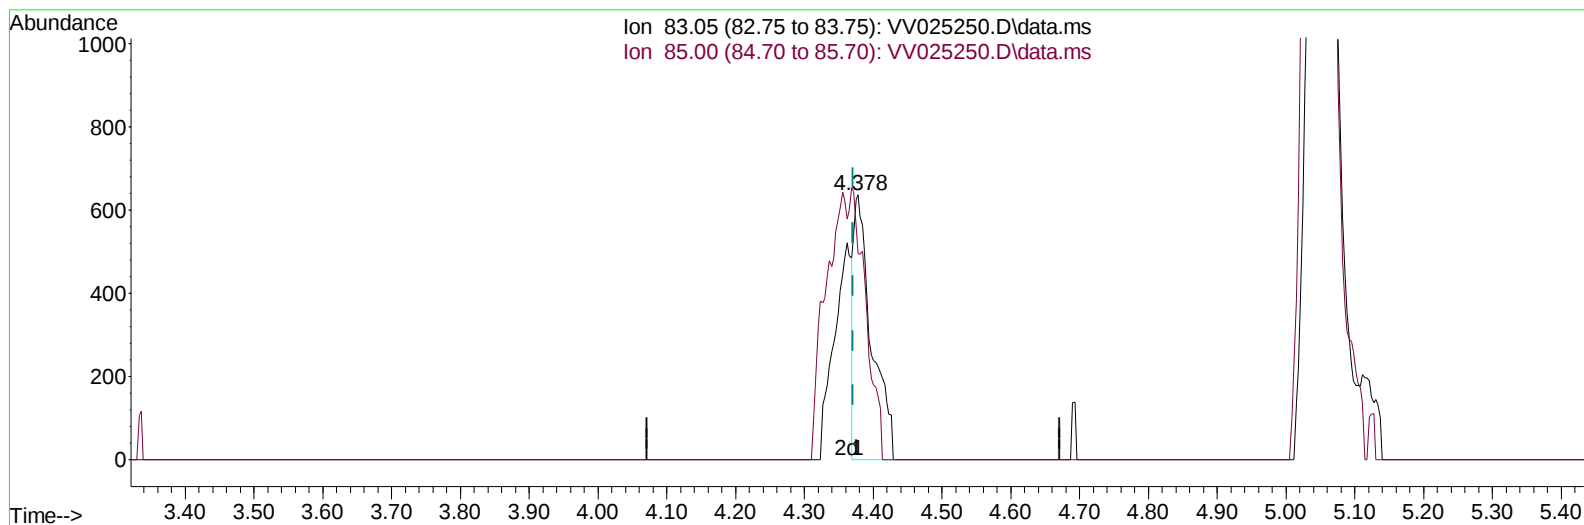

TIC: VV025250.D\data.ms

(25) Chloroform (T)

4.378min (+ 0.007) 0.06 ug/L

response 1159

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	77.83
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025250.D
 Acq On : 28 Mar 2022 10:44
 Operator : SY/MD
 Sample : VV0328wBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/29/2022
 Supervised By :Mahesh Dadoda 04/01/2022

Quant Time: Mar 29 03:40:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration

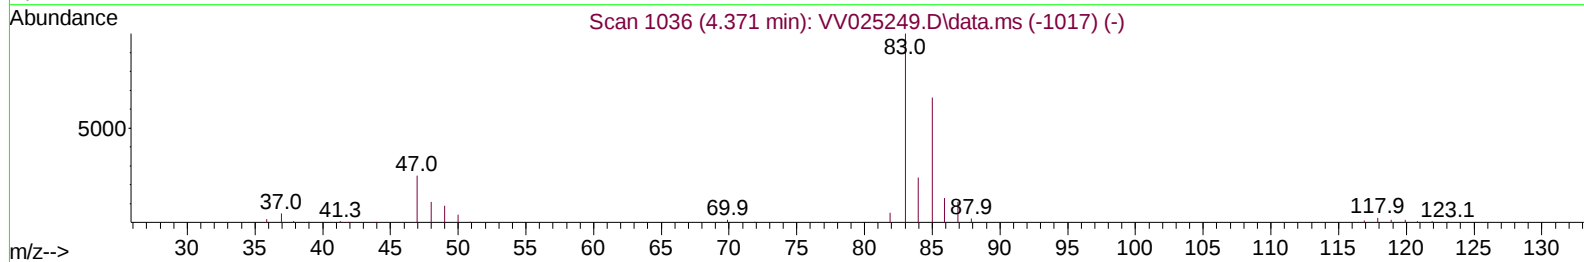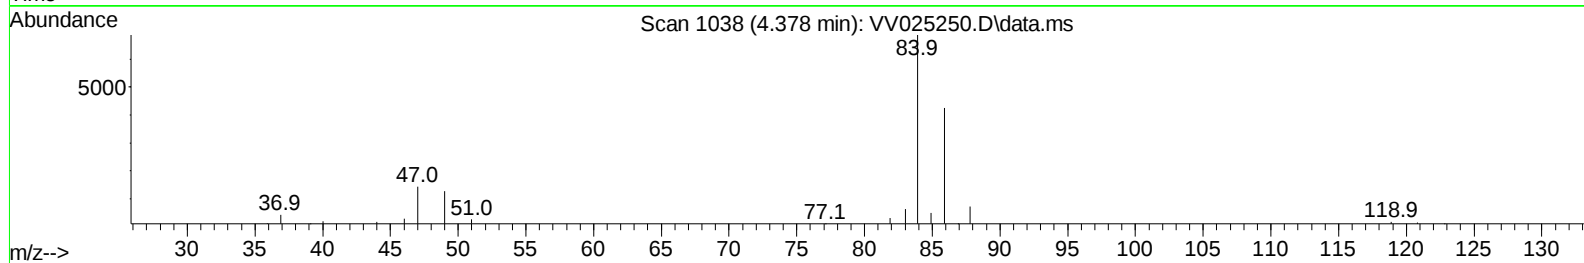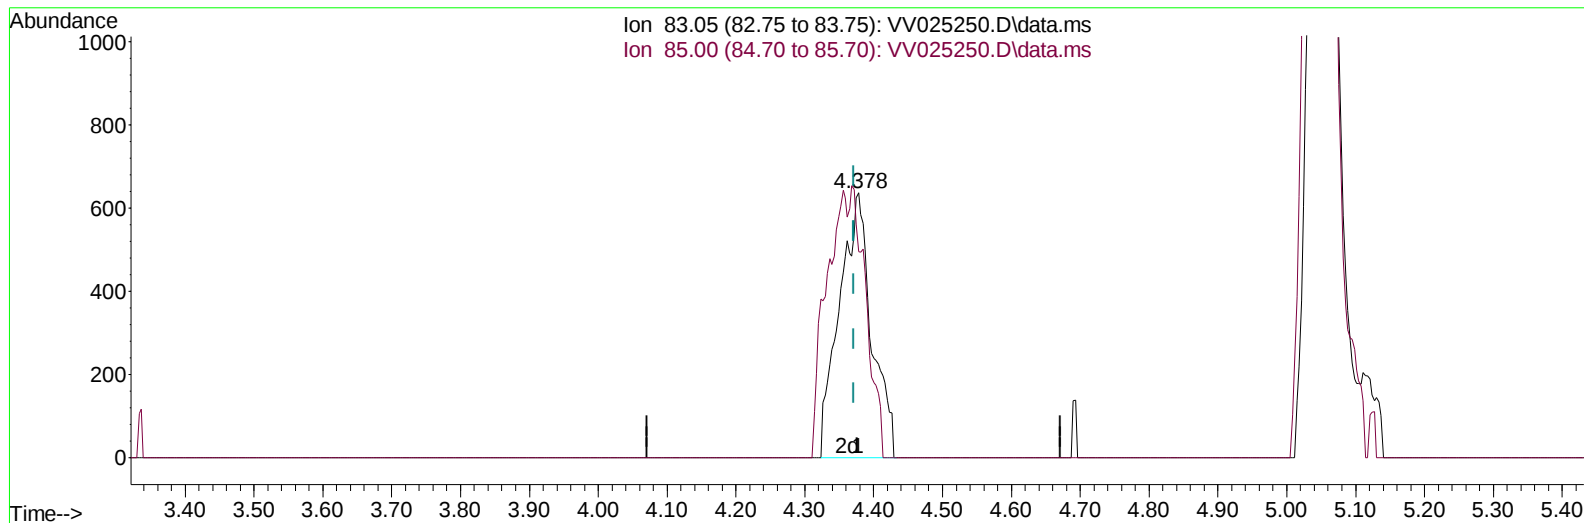

TIC: VV025250.D\data.ms

(25) Chloroform (T)

4.378min (+ 0.007) 0.10 ug/L m

response 2068

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	77.83
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025250.D
 Acq On : 28 Mar 2022 10:44
 Operator : SY/MD
 Sample : VV0328WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 03/29/2022
 Supervised By : Mahesh Dadoda 04/01/2022

Quant Time: Mar 29 03:40:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	154095	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	146065	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	62310	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	65967	4.583	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	91.600%		
7) Chloroethane-d5	1.568	69	59283	4.907	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	98.200%		
11) 1,1-Dichloroethene-d2	2.105	63	112771	3.617	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	72.400%		
20) 2-Butanone-d5	3.915	46	63843	44.528	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	89.060%		
24) Chloroform-d	4.346	84	92092	4.903	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	98.000%		
26) 1,2-Dichloroethane-d4	5.031	65	41479	4.996	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	100.000%		
32) Benzene-d6	5.043	84	188462	5.100	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	102.000%		
36) 1,2-Dichloropropane-d6	6.066	67	53366	5.153	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	103.000%		
41) Toluene-d8	7.310	98	161350	4.760	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	95.200%		
43) trans-1,3-Dichloroprop...	7.622	79	16424	4.861	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	97.200%		
46) 2-Hexanone-d5	8.088	63	59389	48.672	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	97.340%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	34720	5.028	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	100.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152	54044	5.400	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	108.000%		
Target Compounds						Qvalue
25) Chloroform	4.378	83	2068m	0.100	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025250.D
Acq On : 28 Mar 2022 10:44
Operator : SY/MD
Sample : VV0328WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/29/2022
Supervised By :Mahesh Dadoda 04/01/2022

Quant Time: Mar 29 03:40:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

