

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025254.D
 Acq On : 28 Mar 2022 12:25
 Operator : SY/MD
 Sample : N2044-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Mar 29 03:28:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	141579	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	139938	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58115	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	62568	4.731	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.600%
7) Chloroethane-d5	1.567	69	58027	5.228	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.600%
11) 1,1-Dichloroethene-d2	2.104	63	100540	3.510	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.200%
20) 2-Butanone-d5	3.921	46	54430	41.318	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.640%
24) Chloroform-d	4.349	84	89247	5.171	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
26) 1,2-Dichloroethane-d4	5.034	65	41125	5.391	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.800%
32) Benzene-d6	5.050	84	173842	4.910	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
36) 1,2-Dichloropropane-d6	6.069	67	51001	5.140	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.800%
41) Toluene-d8	7.313	98	149966	4.618	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.400%
43) trans-1,3-Dichloroprop...	7.625	79	15268	4.717	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.400%
46) 2-Hexanone-d5	8.091	63	55000	47.049	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.100%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	33255	5.027	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	49737	5.329	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.600%
Target Compounds					Qvalue	
25) Chloroform	4.384	83	2119	0.112	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025254.D
Acq On : 28 Mar 2022 12:25
Operator : SY/MD
Sample : N2044-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Mar 29 03:28:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

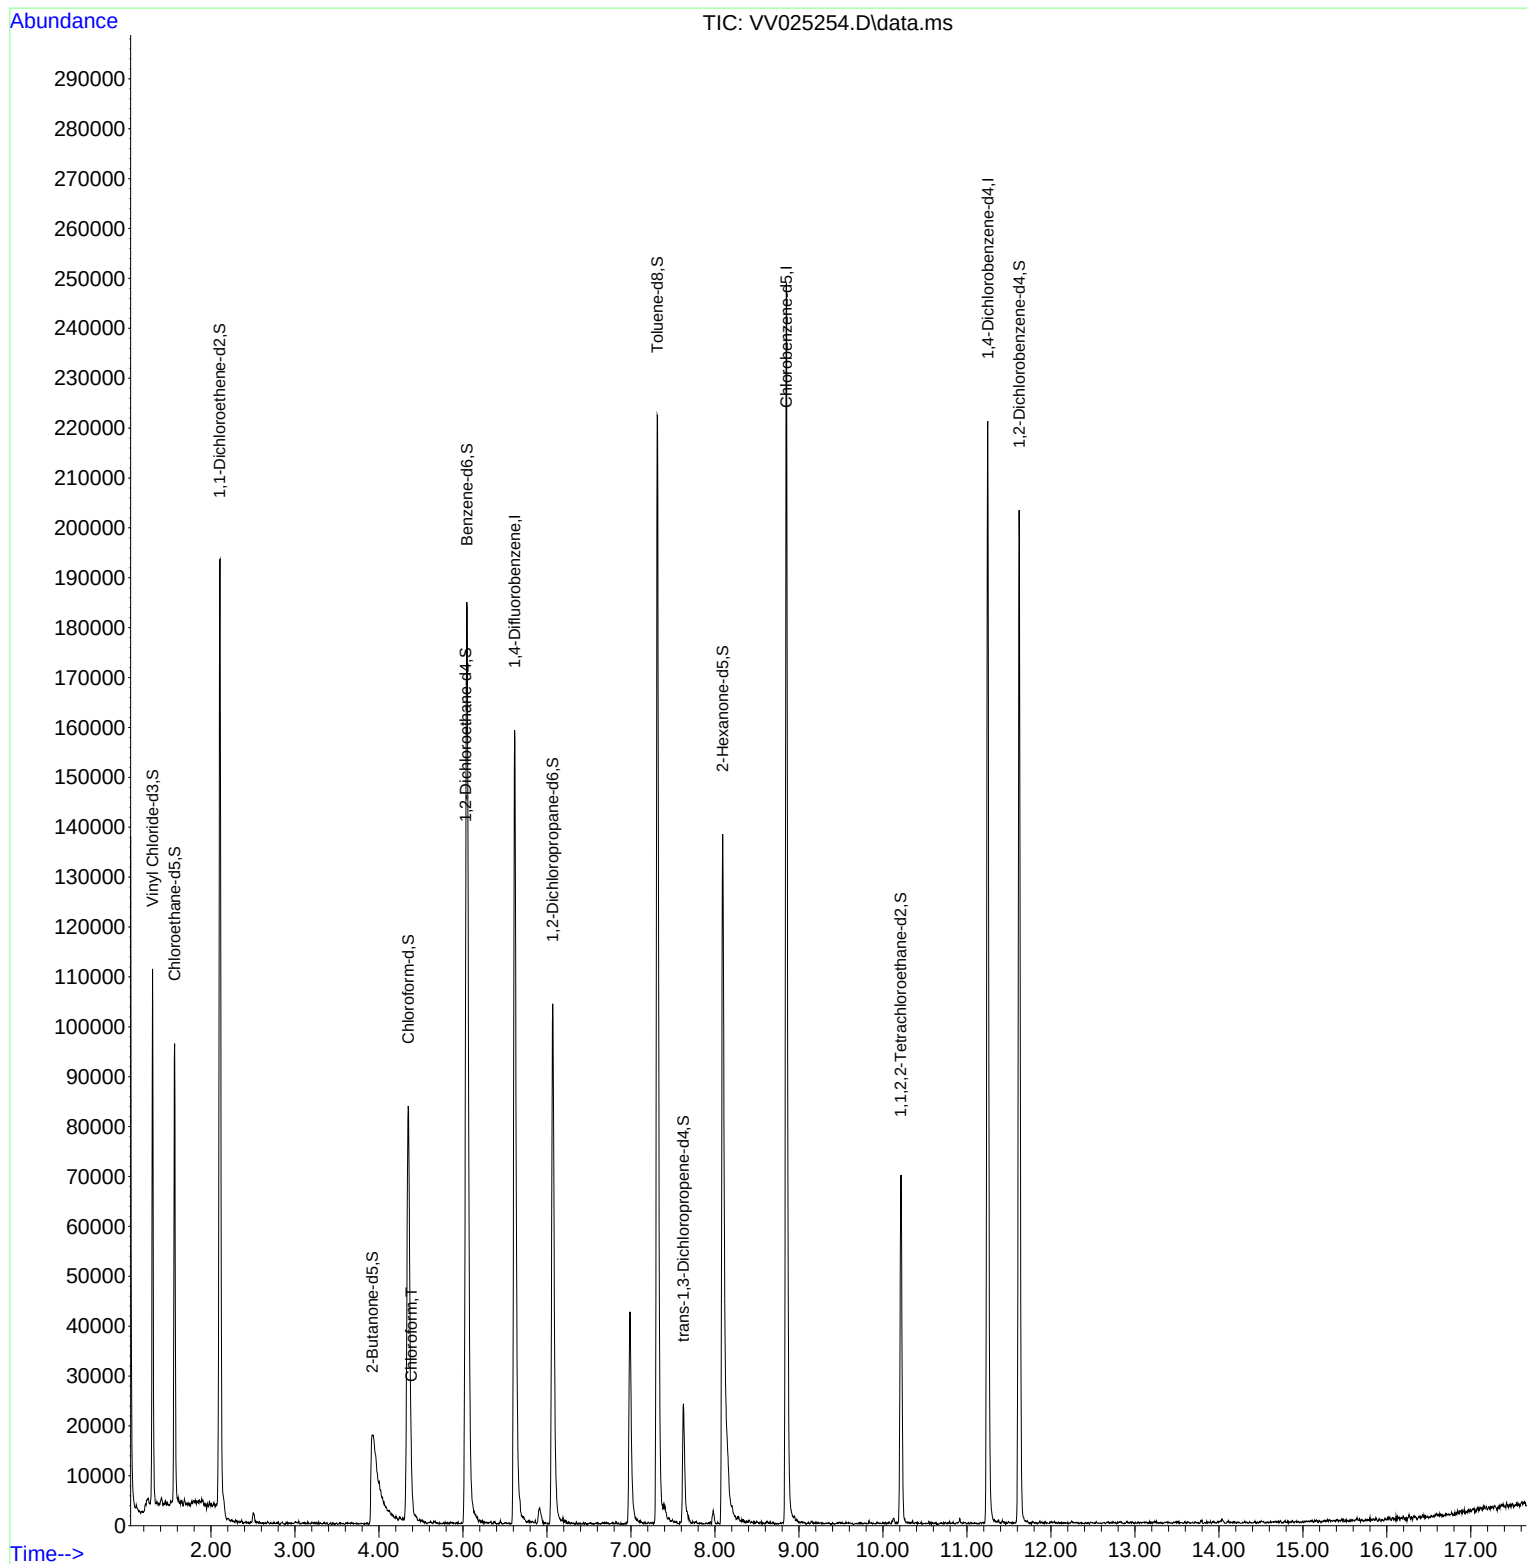

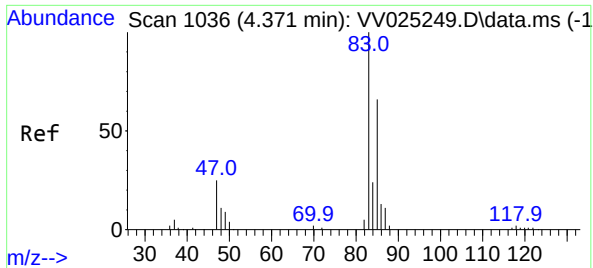

#25
Chloroform
Concen: 0.112 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.013 min
Lab File: VV025254.D
Acq: 28 Mar 2022 12:25

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 83 Resp: 2119
Ion Ratio Lower Upper
83 100
85 62.6 44.7 82.9

