

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032822\
 Data File : VW025259.D
 Acq On : 28 Mar 2022 14:24
 Operator : SY/MD
 Sample : N2110-06DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB6DL

Quant Time: Mar 29 03:29:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	142798	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	140084	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60023	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	62379	4.677	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.600%	
7) Chloroethane-d5	1.568	69	55766	4.981	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.600%	
11) 1,1-Dichloroethene-d2	2.108	63	97609	3.378	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.924	46	49796	37.478	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	74.960%	
24) Chloroform-d	4.349	84	85316	4.901	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	5.034	65	38388	4.989	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.800%	
32) Benzene-d6	5.050	84	168687	4.760	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	6.069	67	49981	5.032	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.600%	
41) Toluene-d8	7.317	98	144591	4.448	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	7.625	79	14403	4.445	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.092	63	54323	46.421	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.840%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32011	4.834	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50326	5.220	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds					Qvalue	
25) Chloroform	4.381	83	2360	0.123	ug/L	90
47) Tetrachloroethene	7.976	164	29591	3.557	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025259.D
Acq On : 28 Mar 2022 14:24
Operator : SY/MD
Sample : N2110-06DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB6DL

Quant Time: Mar 29 03:29:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

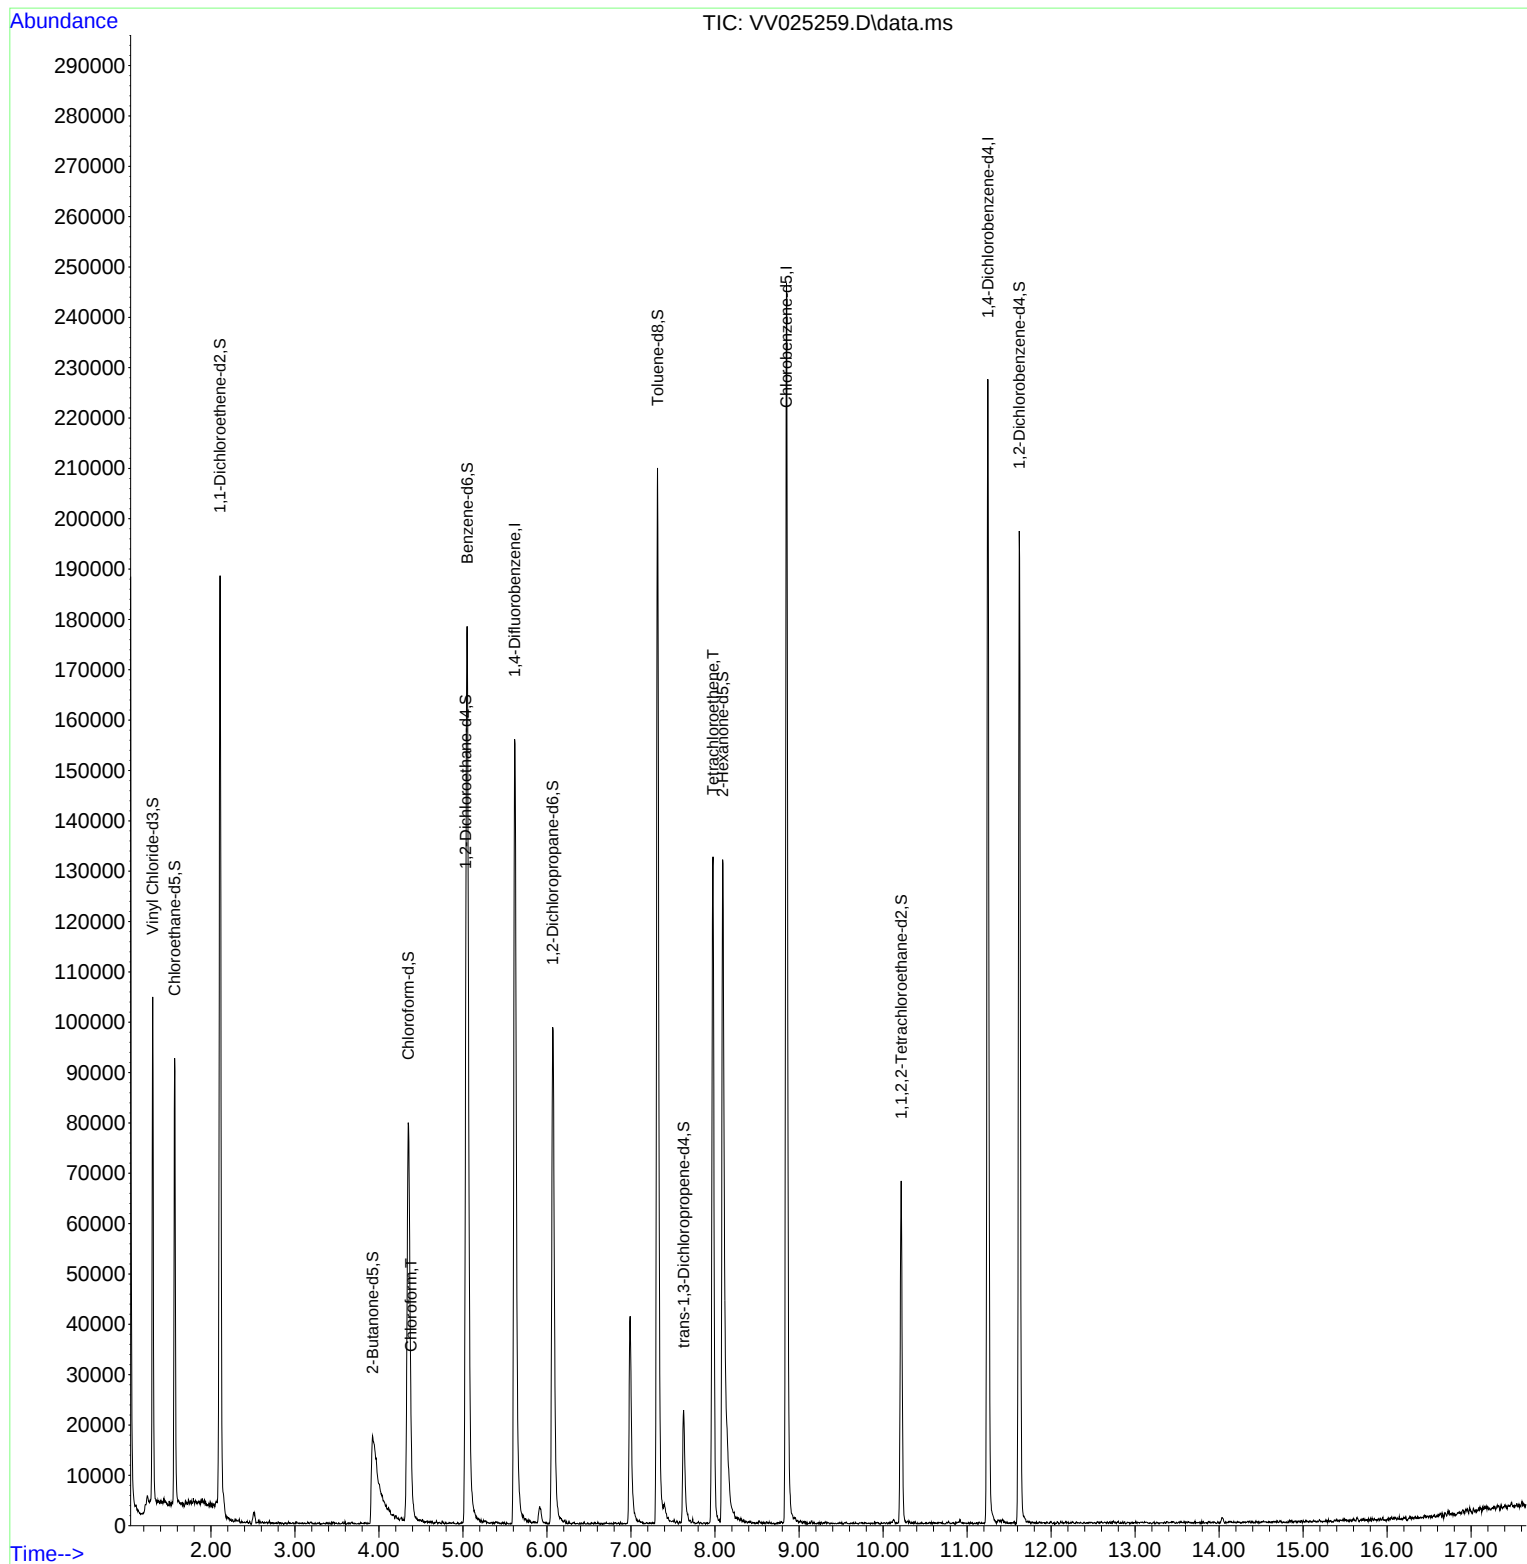

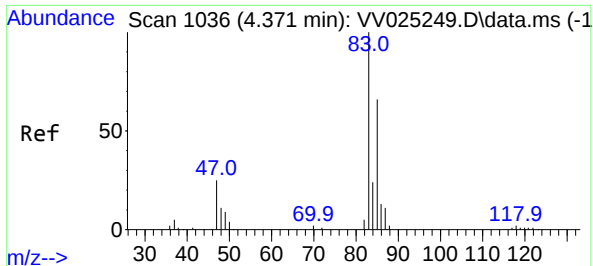

#25

Chloroform

Concen: 0.123 ug/L

RT: 4.381 min Scan# 1036

Delta R.T. 0.010 min

Lab File: VV025259.D

Acq: 28 Mar 2022 14:24

Instrument :

MSVOA_V

ClientSampleId :





C0PB6DL

Tgt Ion: 83 Resp: 2360

Ion Ratio Lower Upper

83 100

85 71.5 44.7 82.9

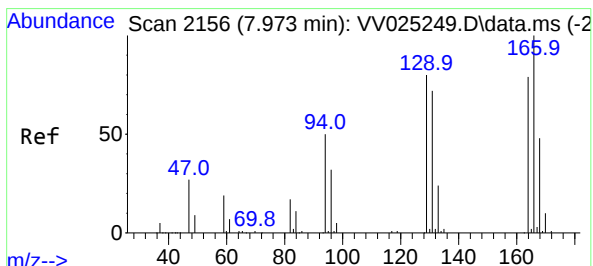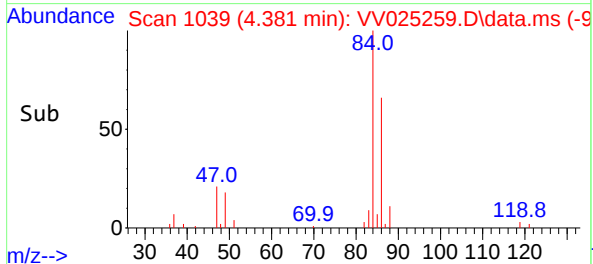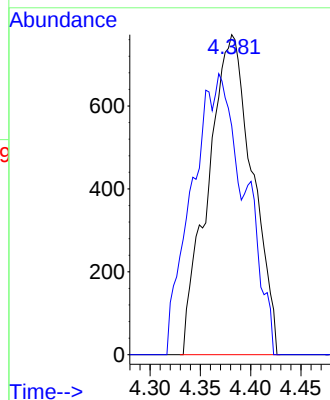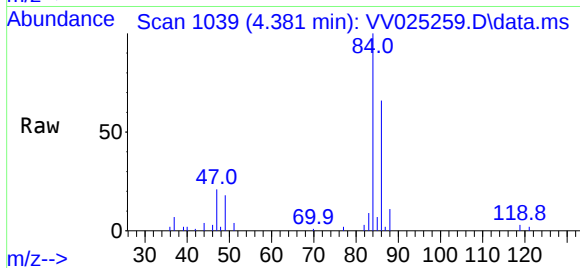

#47

Tetrachloroethene

Concen: 3.557 ug/L

RT: 7.976 min Scan# 2157

Delta R.T. 0.003 min

Lab File: VV025259.D

Acq: 28 Mar 2022 14:24

Tgt Ion: 164 Resp: 29591

Ion Ratio Lower Upper

164 100

129 95.2 67.5 125.4

131 89.4 68.0 126.4

166 123.5 86.2 160.2

