

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032822\
 Data File : VW025261.D
 Acq On : 28 Mar 2022 15:11
 Operator : SY/MD
 Sample : N2110-08DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PC0DL

Quant Time: Mar 29 03:29:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	147158	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	143737	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64094	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	61311	4.460	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.200%
7) Chloroethane-d5	1.568	69	56304	4.880	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.600%
11) 1,1-Dichloroethene-d2	2.108	63	99359	3.337	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.800%
20) 2-Butanone-d5	3.921	46	60494	44.181	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.360%
24) Chloroform-d	4.352	84	88450	4.931	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
26) 1,2-Dichloroethane-d4	5.034	65	40642	5.126	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.050	84	178214	4.901	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
36) 1,2-Dichloropropane-d6	6.069	67	50376	4.943	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.800%
41) Toluene-d8	7.316	98	152540	4.573	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
43) trans-1,3-Dichloroprop...	7.625	79	14613	4.395	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.000%
46) 2-Hexanone-d5	8.091	63	57121	47.571	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.140%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	33983	5.001	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	52159	5.067	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%
Target Compounds						Qvalue
25) Chloroform	4.381	83	2453	0.125	ug/L	81
47) Tetrachloroethene	7.976	164	33411	3.914	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025261.D
Acq On : 28 Mar 2022 15:11
Operator : SY/MD
Sample : N2110-08DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC0DL

Quant Time: Mar 29 03:29:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

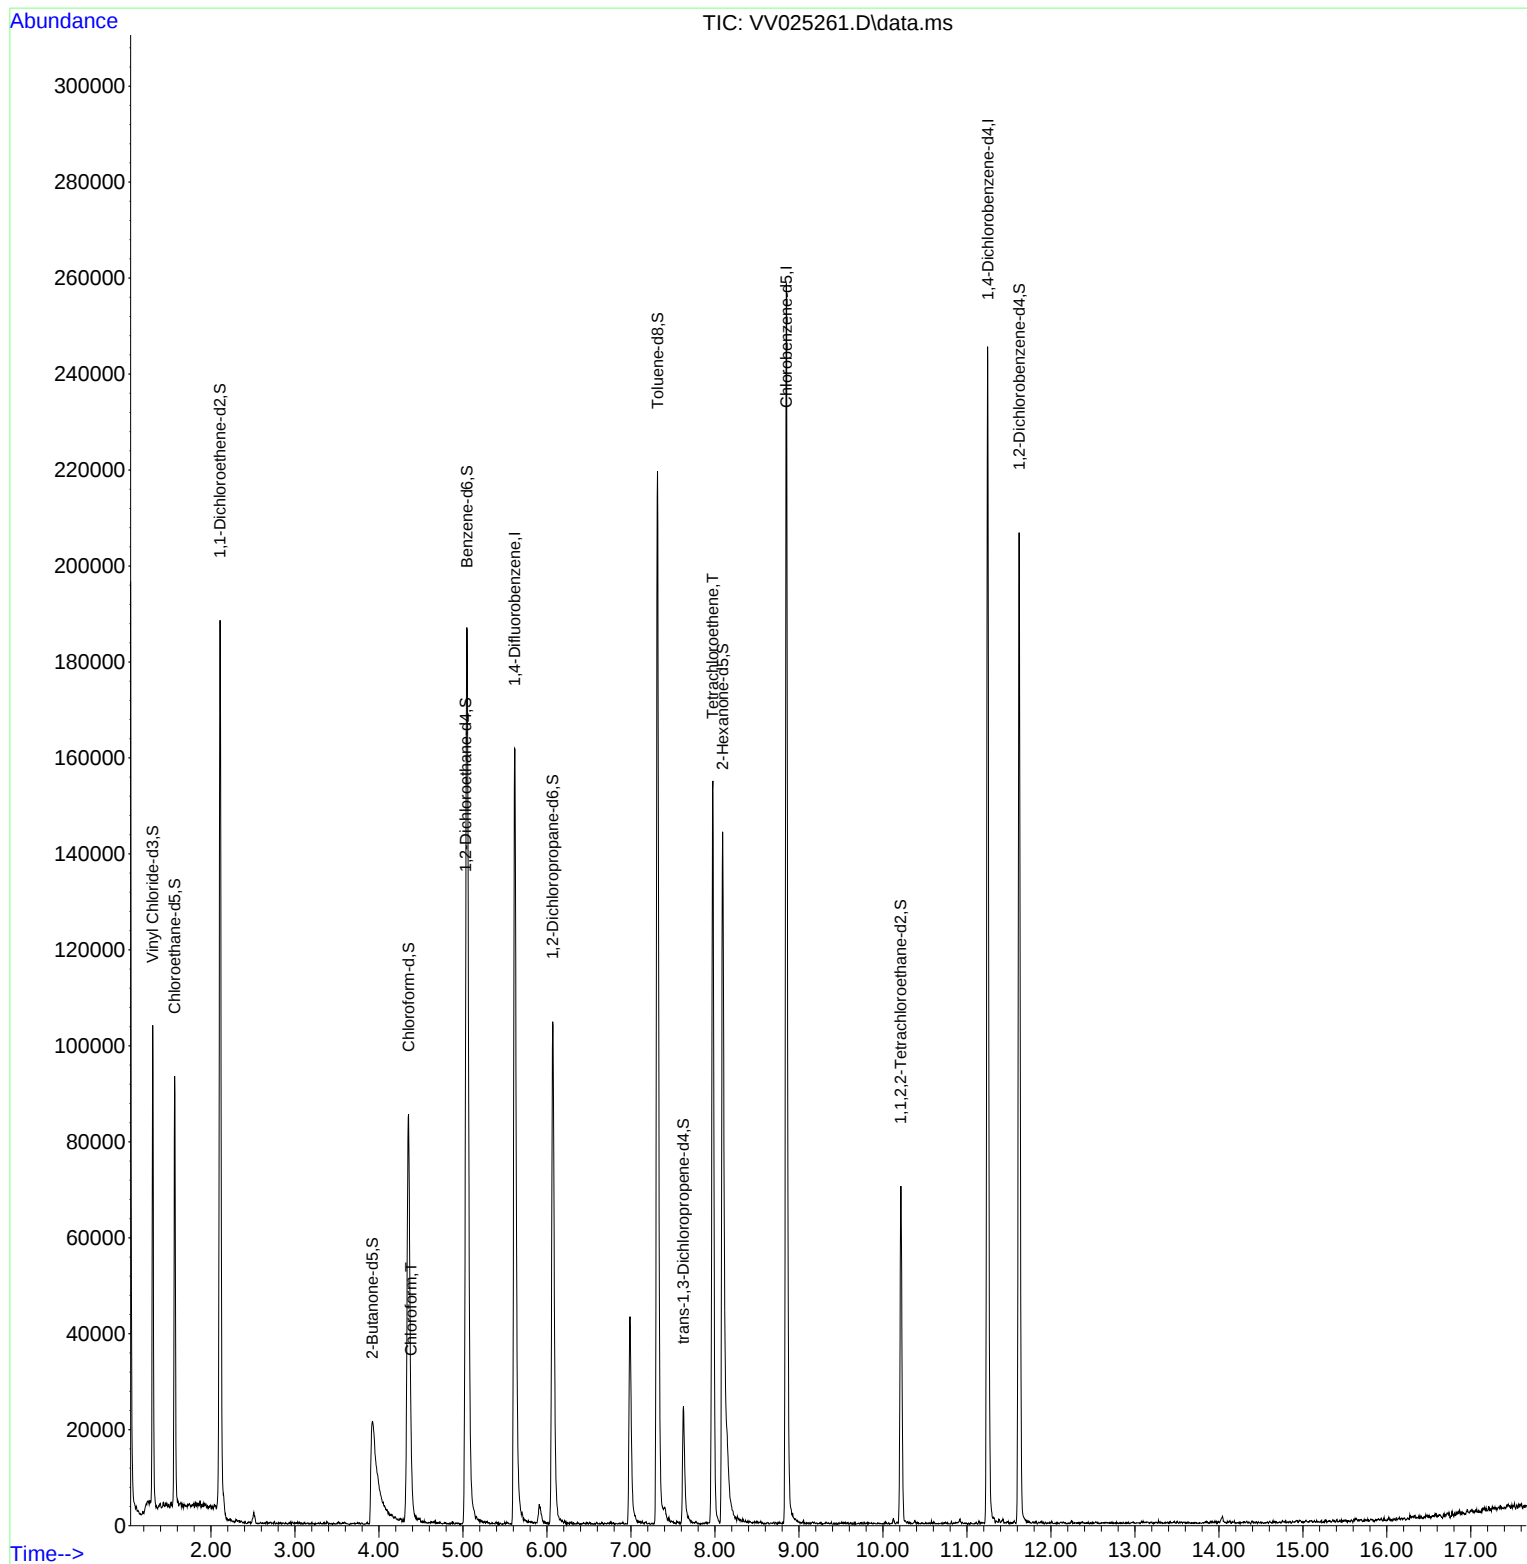

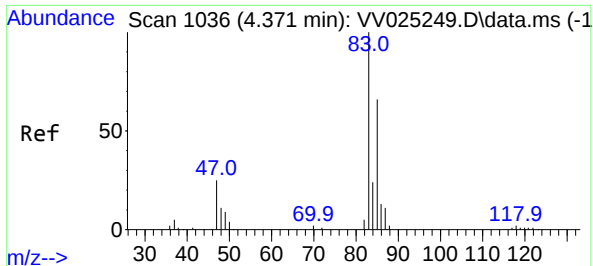

#25

Chloroform

Concen: 0.125 ug/L

RT: 4.381 min Scan# 1036

Delta R.T. 0.010 min

Lab File: VV025261.D

Acq: 28 Mar 2022 15:11

Instrument :

MSVOA_V

ClientSampleId :





C0PC0DL

Tgt Ion: 83 Resp: 2453

Ion Ratio Lower Upper

83 100

85 78.4 44.7 82.9

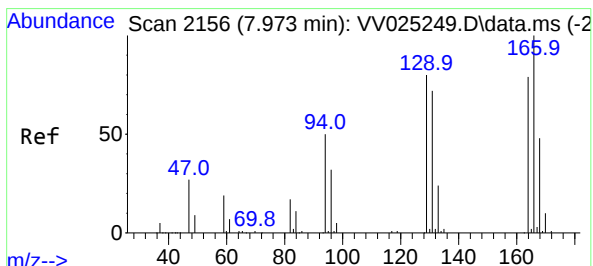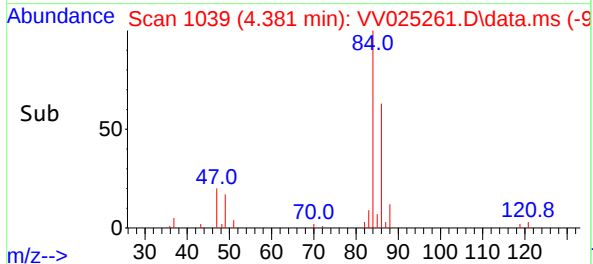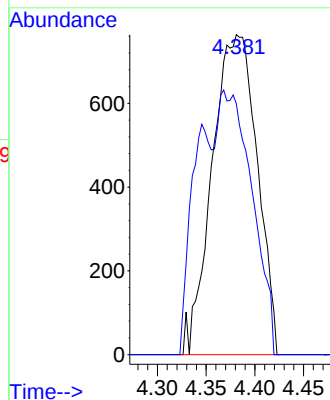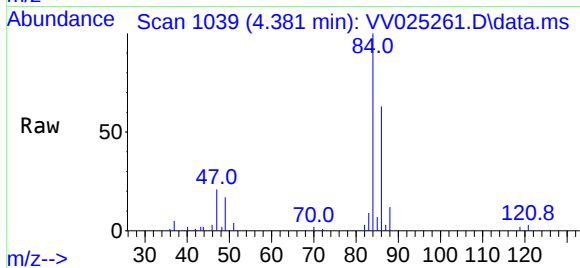

#47

Tetrachloroethene

Concen: 3.914 ug/L

RT: 7.976 min Scan# 2157

Delta R.T. 0.003 min

Lab File: VV025261.D

Acq: 28 Mar 2022 15:11

Tgt Ion: 164 Resp: 33411

Ion Ratio Lower Upper

164 100

129 97.1 67.5 125.4

131 93.4 68.0 126.4

166 128.8 86.2 160.2

