

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032822\
 Data File : VW025264.D
 Acq On : 28 Mar 2022 16:21
 Operator : SY/MD
 Sample : N2110-13DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PD2DL

Quant Time: Mar 29 03:30:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	144446	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	143491	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60121	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59798	4.432	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.600%	
7) Chloroethane-d5	1.568	69	54303	4.795	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.108	63	99285	3.397	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.000%	
20) 2-Butanone-d5	3.918	46	53034	39.460	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	78.920%	
24) Chloroform-d	4.349	84	84148	4.779	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
26) 1,2-Dichloroethane-d4	5.034	65	39162	5.032	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.600%	
32) Benzene-d6	5.050	84	172371	4.748	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.000%	
36) 1,2-Dichloropropane-d6	6.069	67	48953	4.812	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.200%	
41) Toluene-d8	7.317	98	145390	4.366	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.400%	
43) trans-1,3-Dichloroprop...	7.625	79	13744	4.141	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.800%	
46) 2-Hexanone-d5	8.092	63	53083	44.284	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.560%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31830	4.692	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	49856	5.163	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.200%	
Target Compounds						
25) Chloroform	4.384	83	2864	0.148	ug/L	90
47) Tetrachloroethene	7.976	164	37729	4.427	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025264.D
Acq On : 28 Mar 2022 16:21
Operator : SY/MD
Sample : N2110-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PD2DL

Quant Time: Mar 29 03:30:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

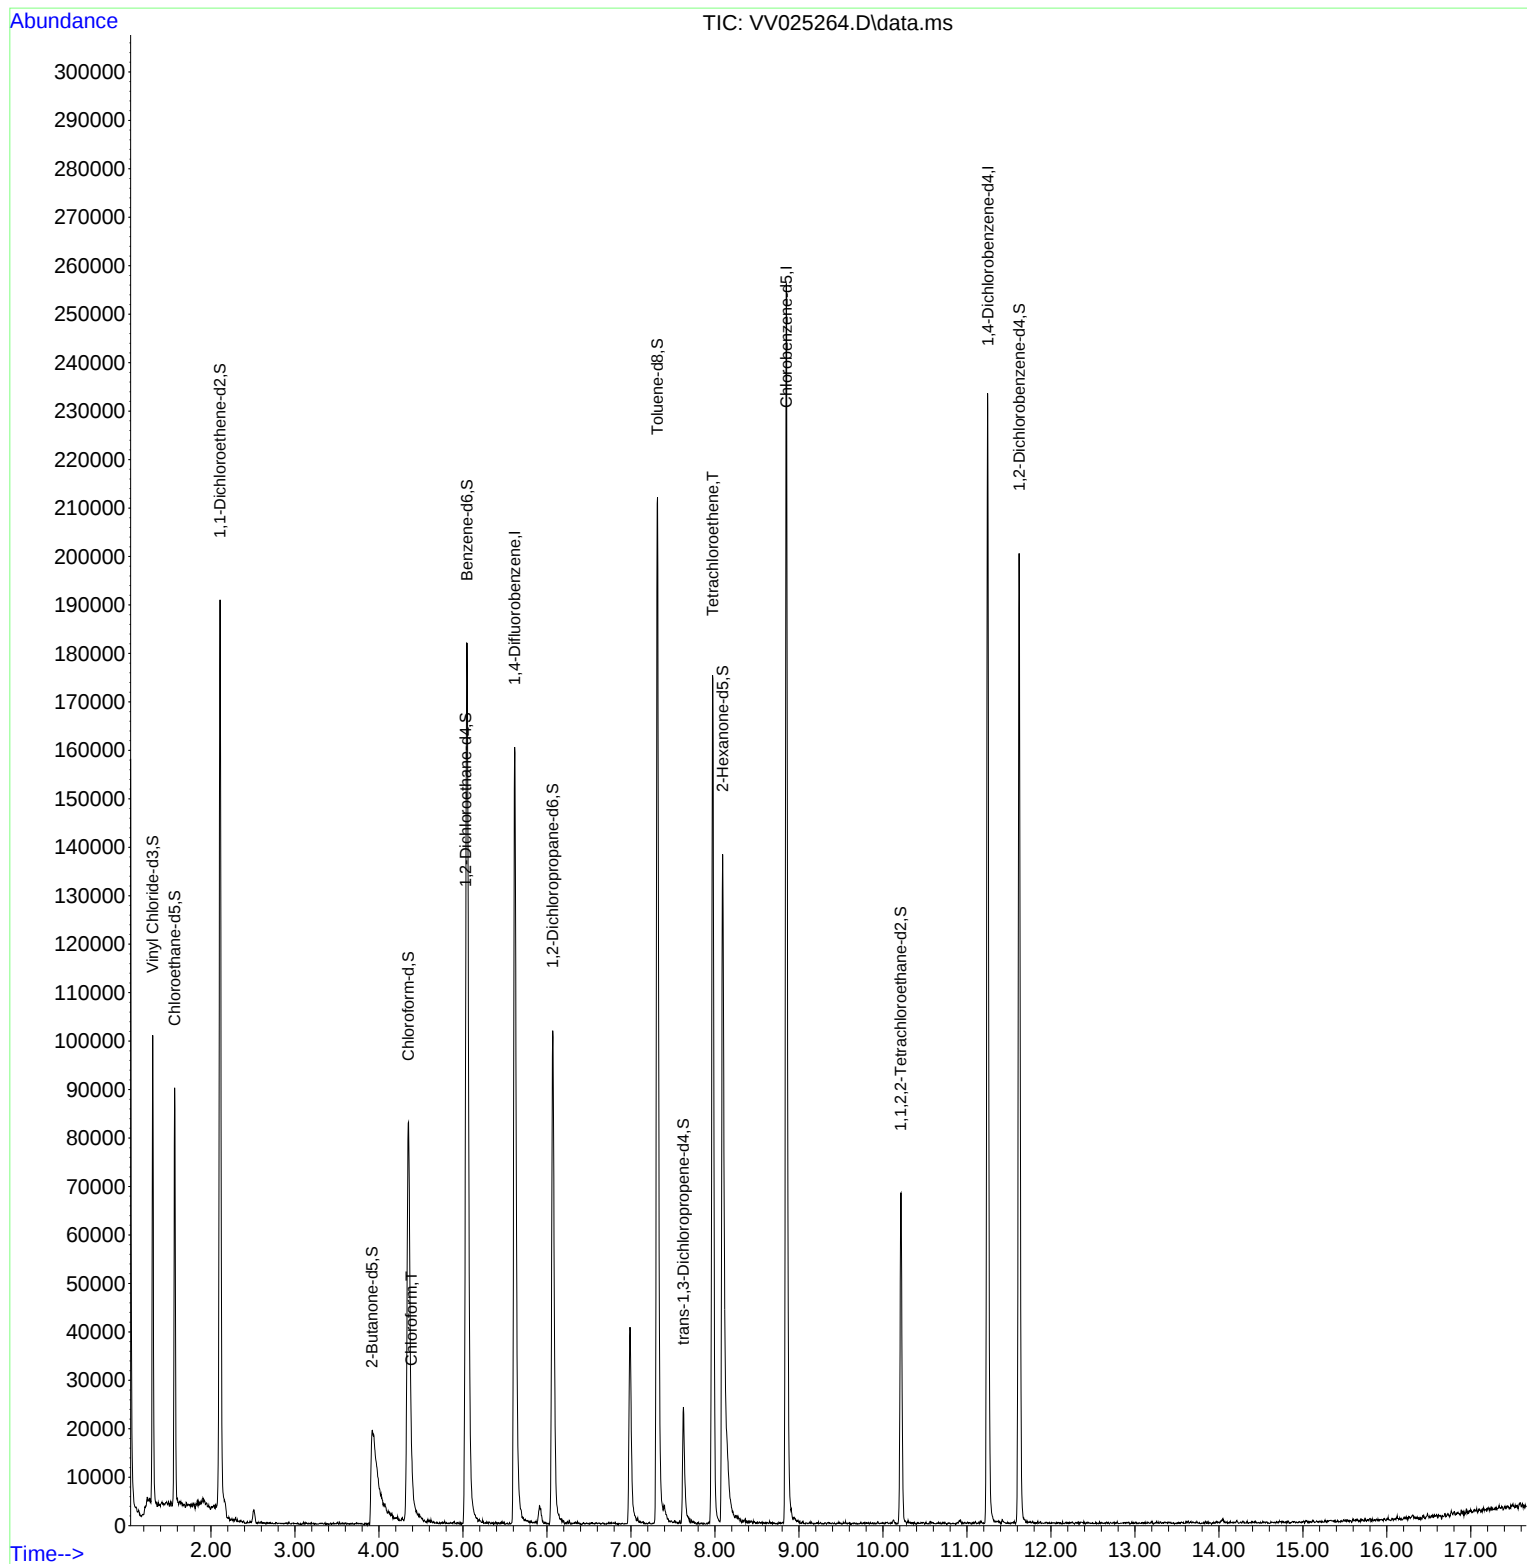

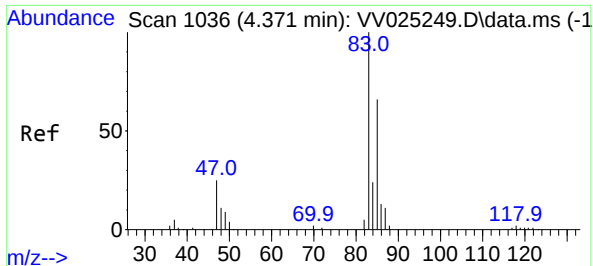

#25

Chloroform

Concen: 0.148 ug/L

RT: 4.384 min Scan# 1036

Delta R.T. 0.013 min

Lab File: VV025264.D

Acq: 28 Mar 2022 16:21

Instrument :

MSVOA_V

ClientSampleId :





C0PD2DL

Tgt Ion: 83 Resp: 2864

Ion Ratio Lower Upper

83 100

85 55.8 44.7 82.9

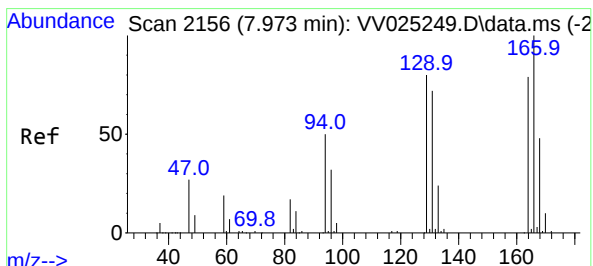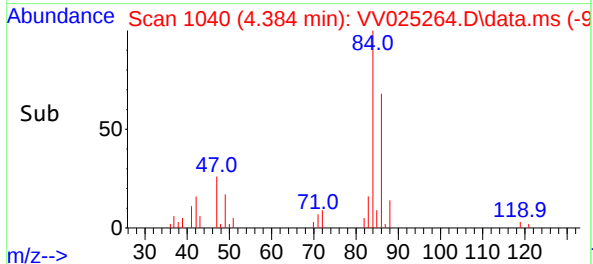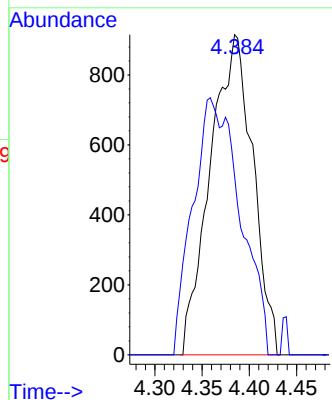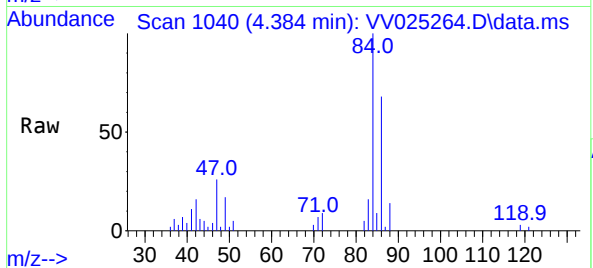

#47

Tetrachloroethene

Concen: 4.427 ug/L

RT: 7.976 min Scan# 2157

Delta R.T. 0.003 min

Lab File: VV025264.D

Acq: 28 Mar 2022 16:21

Tgt Ion: 164 Resp: 37729

Ion Ratio Lower Upper

164 100

129 99.3 67.5 125.4

131 95.1 68.0 126.4

166 131.5 86.2 160.2

