

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032822\
 Data File : VW025267.D
 Acq On : 28 Mar 2022 17:31
 Operator : SY/MD
 Sample : N2101-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAYW8

Quant Time: Mar 29 03:30:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	142248	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	140355	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56542	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	54776	4.122	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.400%
7) Chloroethane-d5	1.568	69	49547	4.443	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.800%
11) 1,1-Dichloroethene-d2	2.108	63	87559	3.042	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.800%
20) 2-Butanone-d5	3.912	46	62549	47.258	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.520%
24) Chloroform-d	4.349	84	83283	4.803	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
26) 1,2-Dichloroethane-d4	5.037	65	37996	4.957	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.050	84	164789	4.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%
36) 1,2-Dichloropropane-d6	6.069	67	48309	4.855	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.317	98	139878	4.295	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%
43) trans-1,3-Dichloroprop...	7.625	79	13085	4.031	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.600%
46) 2-Hexanone-d5	8.092	63	52933	45.146	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.300%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32727	4.932	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	49254	5.424	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.400%
Target Compounds						
14) Carbon disulfide	2.298	76	2034	0.069	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025267.D
Acq On : 28 Mar 2022 17:31
Operator : SY/MD
Sample : N2101-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW8


Quant Time: Mar 29 03:30:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

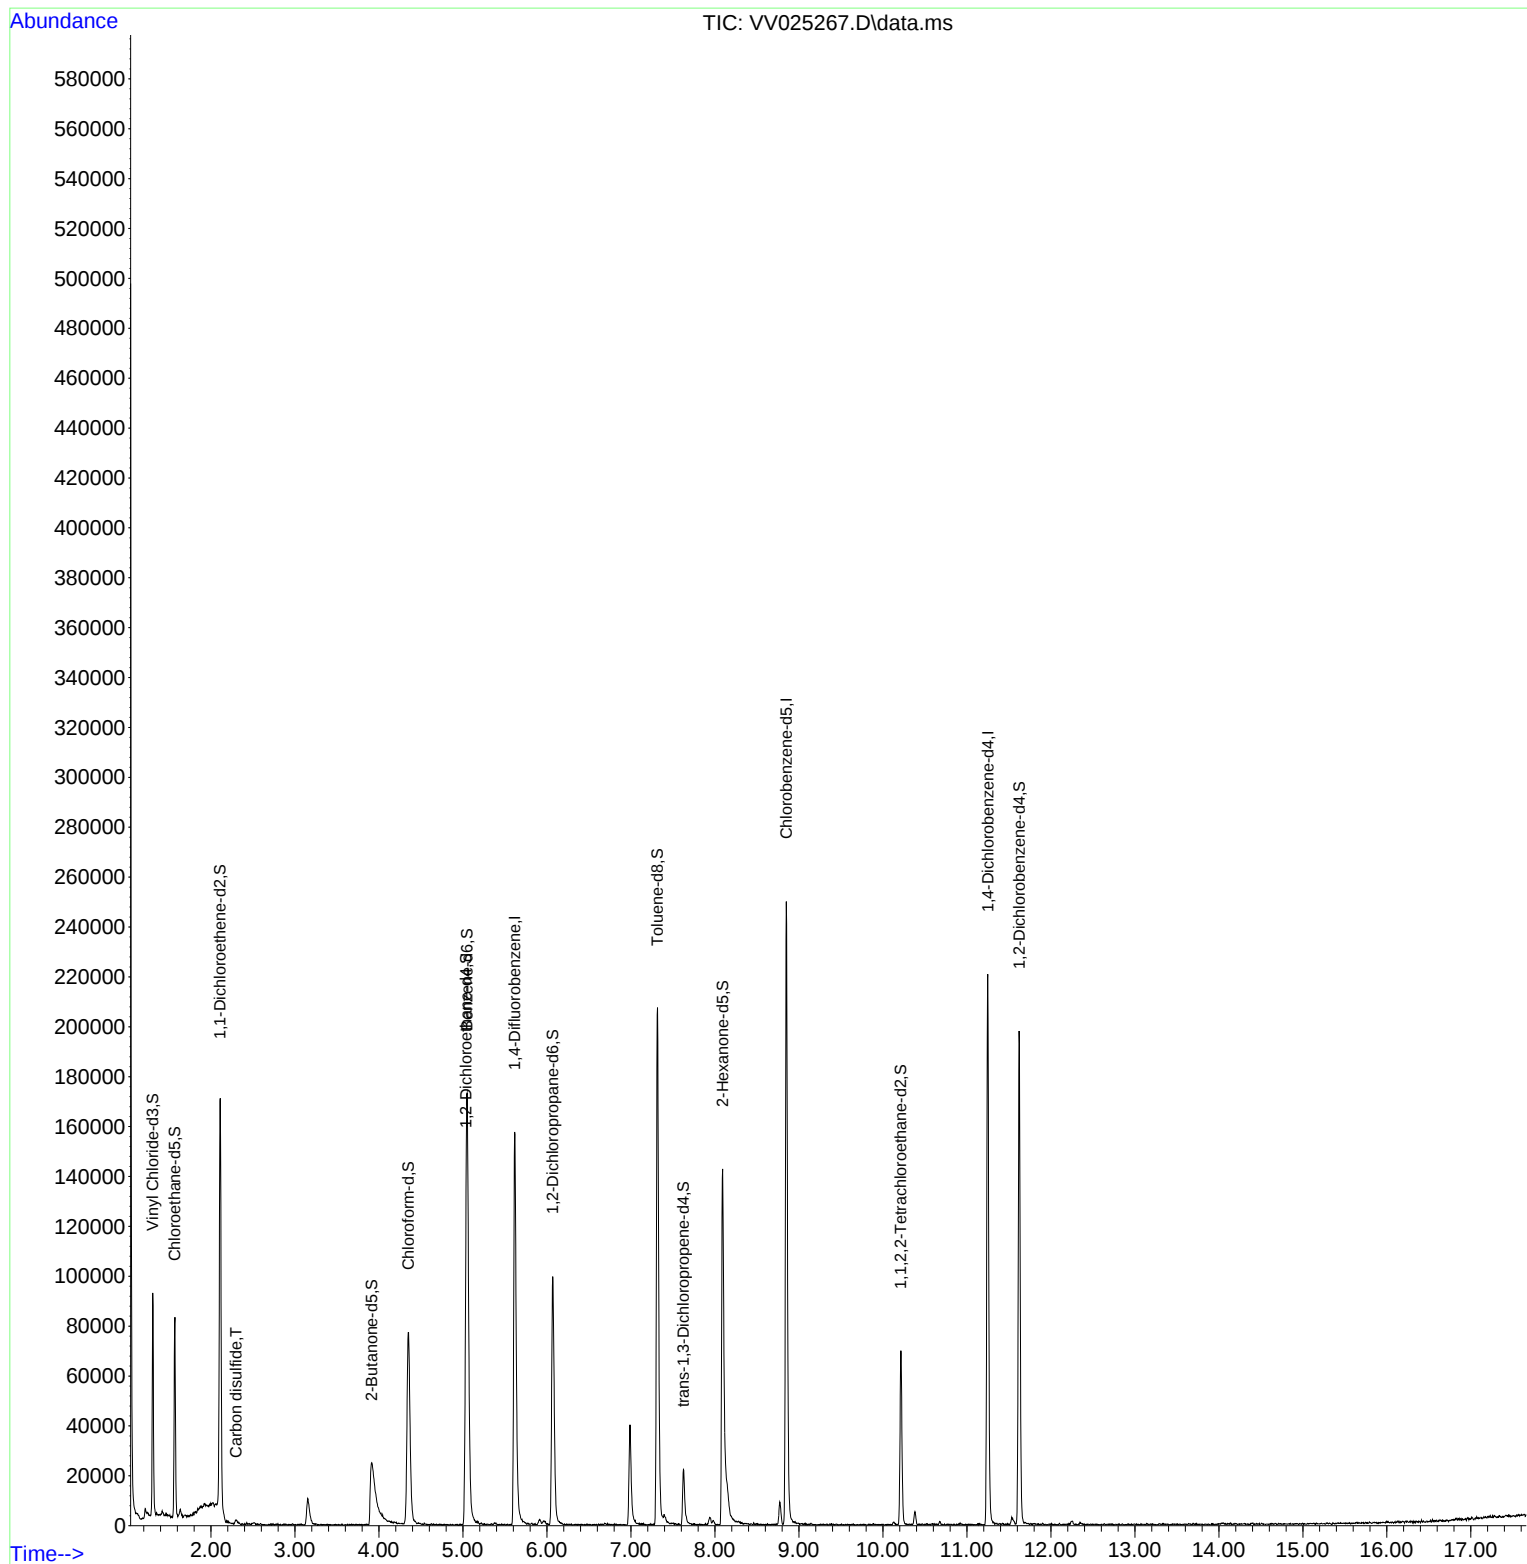

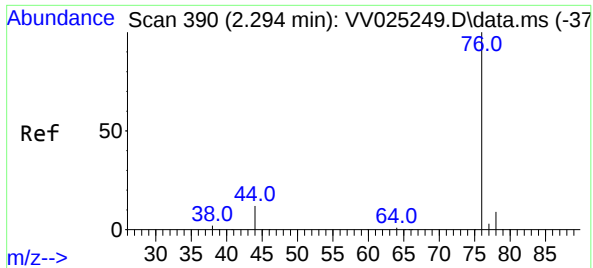

#14
Carbon disulfide
Concen: 0.069 ug/L
RT: 2.298 min Scan# 391
Delta R.T. 0.003 min
Lab File: VV025267.D
Acq: 28 Mar 2022 17:31

Instrument :
MSVOA_V
ClientSampleId :
YAYW8

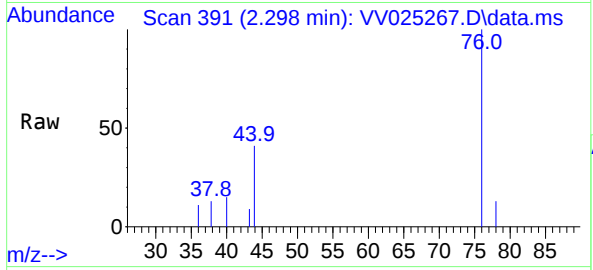

Tgt Ion: 76 Resp: 2034
Ion Ratio Lower Upper
76 100
78 12.9 7.0 10.4#

