

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032822\
 Data File : VW025270.D
 Acq On : 28 Mar 2022 18:41
 Operator : SY/MD
 Sample : N2101-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAZ50

Quant Time: Mar 29 03:31:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 03:26:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	142617	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	141557	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	59981	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	52180	3.917	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.400%
7) Chloroethane-d5	1.571	69	50597	4.525	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.111	63	86319	2.991	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.800%#
20) 2-Butanone-d5	3.896	46	58111	43.792	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.580%
24) Chloroform-d	4.352	84	85640	4.926	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
26) 1,2-Dichloroethane-d4	5.034	65	39616	5.155	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	5.053	84	168452	4.704	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	6.069	67	49958	4.978	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.317	98	144184	4.389	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	7.625	79	13172	4.023	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.088	63	50056	42.330	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.660%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32287	4.825	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	49402	5.128	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds						Qvalue
14) Carbon disulfide	2.301	76	3949	0.133	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025270.D
Acq On : 28 Mar 2022 18:41
Operator : SY/MD
Sample : N2101-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ50

Quant Time: Mar 29 03:31:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 03:26:38 2022
Response via : Initial Calibration

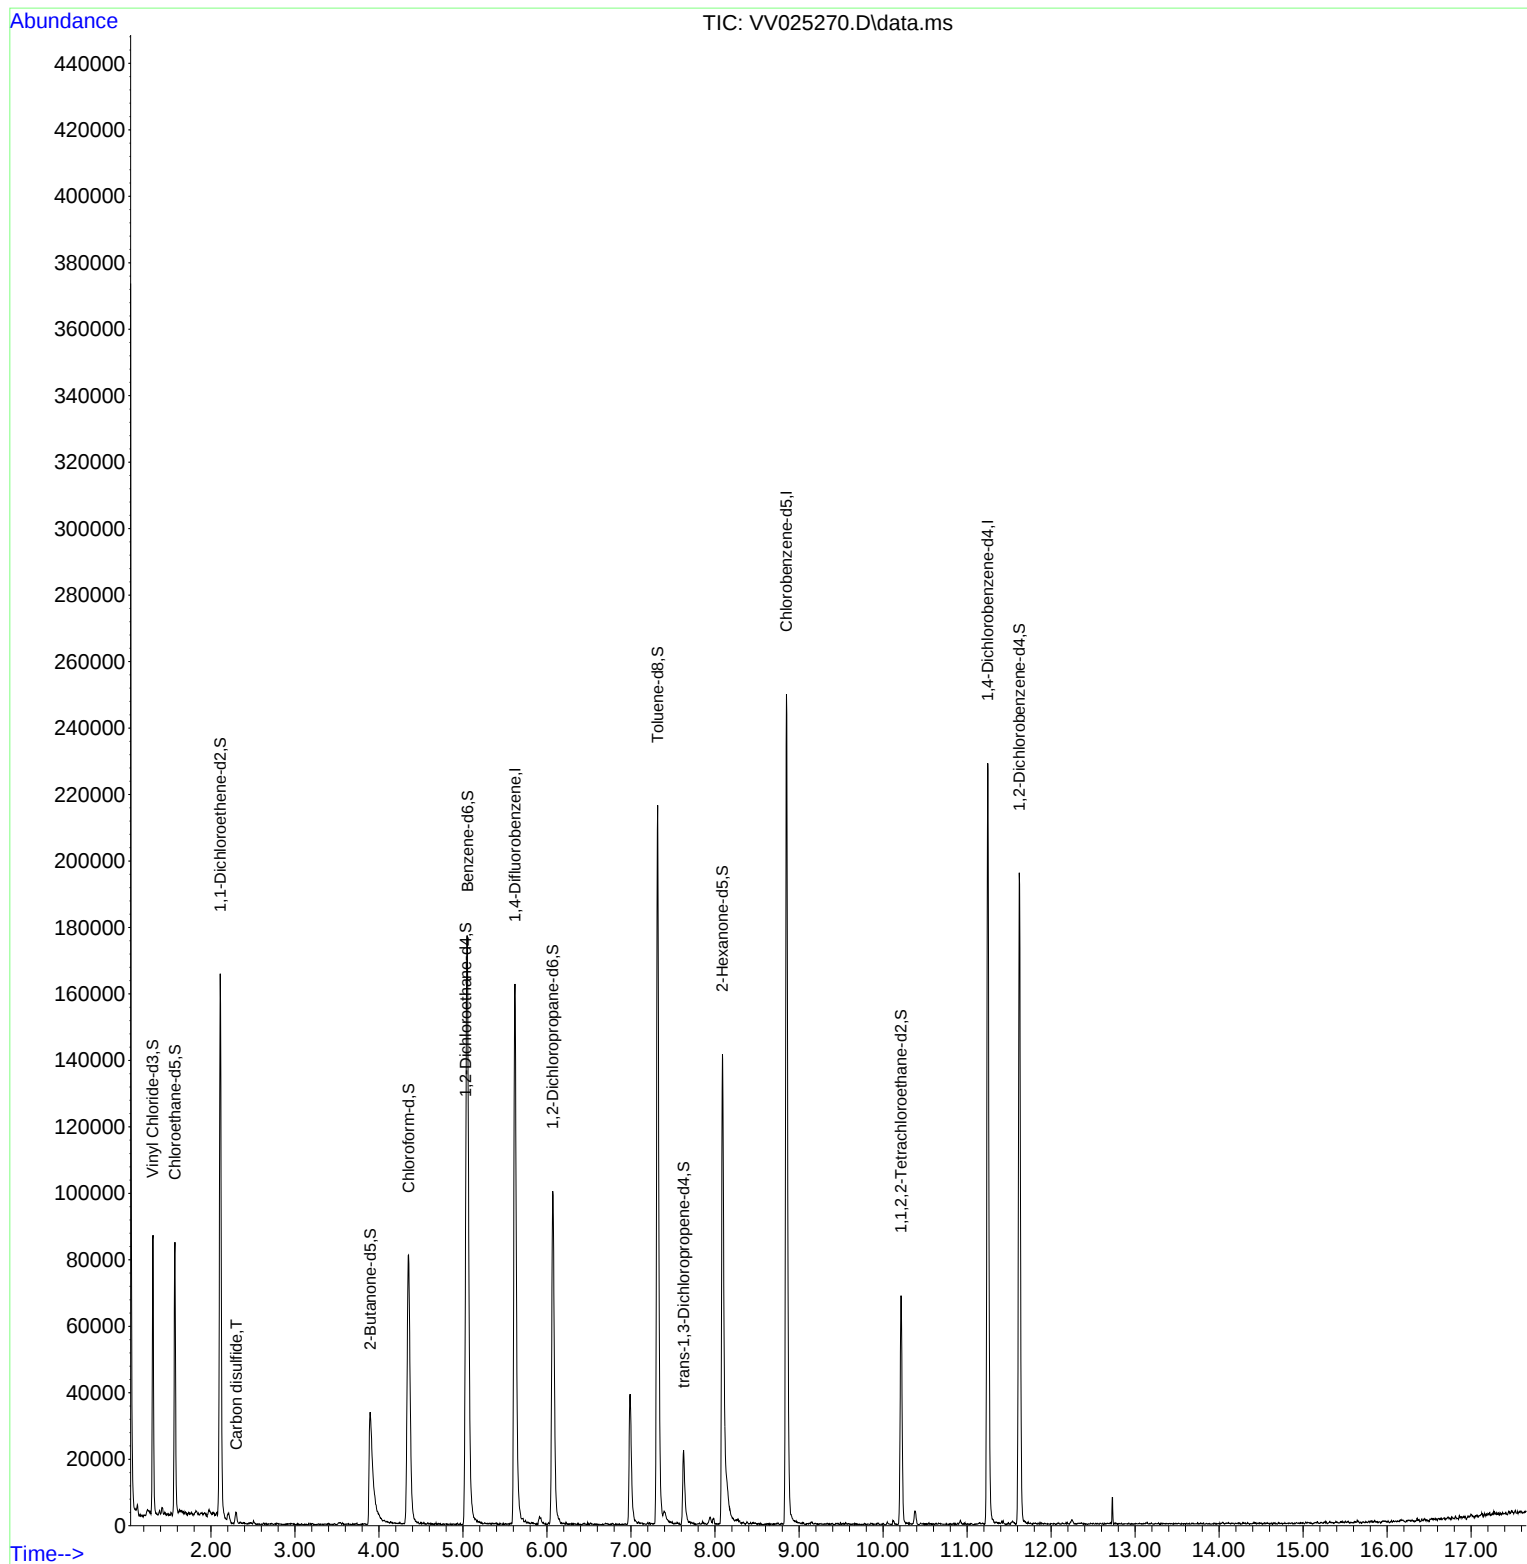

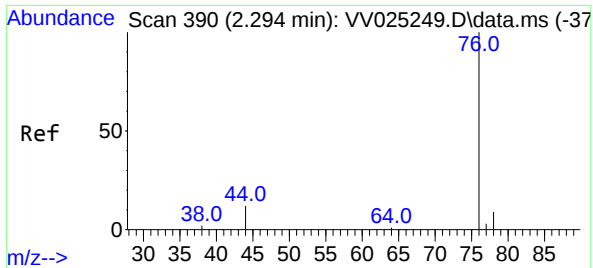

#14
Carbon disulfide
Concen: 0.133 ug/L
RT: 2.301 min Scan# 392
Delta R.T. 0.006 min
Lab File: VV025270.D
Acq: 28 Mar 2022 18:41

Instrument :
MSVOA_V
ClientSampleId :
YAZ50

Tgt Ion: 76 Resp: 3949
Ion Ratio Lower Upper
76 100
78 7.1 7.0 10.4

