

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW032822\  
 Data File : VW025271.D  
 Acq On : 28 Mar 2022 19:04  
 Operator : SY/MD  
 Sample : N2101-10  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 YAZ52

Quant Time: Mar 29 03:31:38 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR032622WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Tue Mar 29 03:26:38 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon           | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|----------------|----------|--------|----------|----------|
| -----                         |        |                |          |        |          |          |
| Internal Standards            |        |                |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.619  | 114            | 140044   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.854  | 117            | 137615   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152            | 57156    | 5.000  | ug/L     | 0.00     |
|                               |        |                |          |        |          |          |
| System Monitoring Compounds   |        |                |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.307  | 65             | 51651    | 3.948  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 79.000%  |          |
| 7) Chloroethane-d5            | 1.571  | 69             | 50699    | 4.618  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 92.400%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.111  | 63             | 84059    | 2.967  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 59.400%# |          |
| 20) 2-Butanone-d5             | 3.892  | 46             | 64505    | 49.503 | ug/L     | -0.02    |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 99.000%  |          |
| 24) Chloroform-d              | 4.349  | 84             | 86801    | 5.085  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 101.600% |          |
| 26) 1,2-Dichloroethane-d4     | 5.034  | 65             | 38608    | 5.117  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 102.400% |          |
| 32) Benzene-d6                | 5.053  | 84             | 172184   | 4.946  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 99.000%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.069  | 67             | 50739    | 5.200  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 104.000% |          |
| 41) Toluene-d8                | 7.317  | 98             | 147269   | 4.612  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 92.200%  |          |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79             | 13106    | 4.117  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 82.400%  |          |
| 46) 2-Hexanone-d5             | 8.088  | 63             | 50987    | 44.352 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 88.700%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.214 | 84             | 33042    | 5.079  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 101.600% |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152            | 50265    | 5.476  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 109.600% |          |
|                               |        |                |          |        |          |          |
| Target Compounds              |        |                |          |        |          | Qvalue   |
| 14) Carbon disulfide          | 2.301  | 76             | 2204     | 0.075  | ug/L     | 97       |
| -----                         |        |                |          |        |          |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV032822\  
Data File : VV025271.D  
Acq On : 28 Mar 2022 19:04  
Operator : SY/MD  
Sample : N2101-10  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
YAZ52

Quant Time: Mar 29 03:31:38 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR032622WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Tue Mar 29 03:26:38 2022  
Response via : Initial Calibration

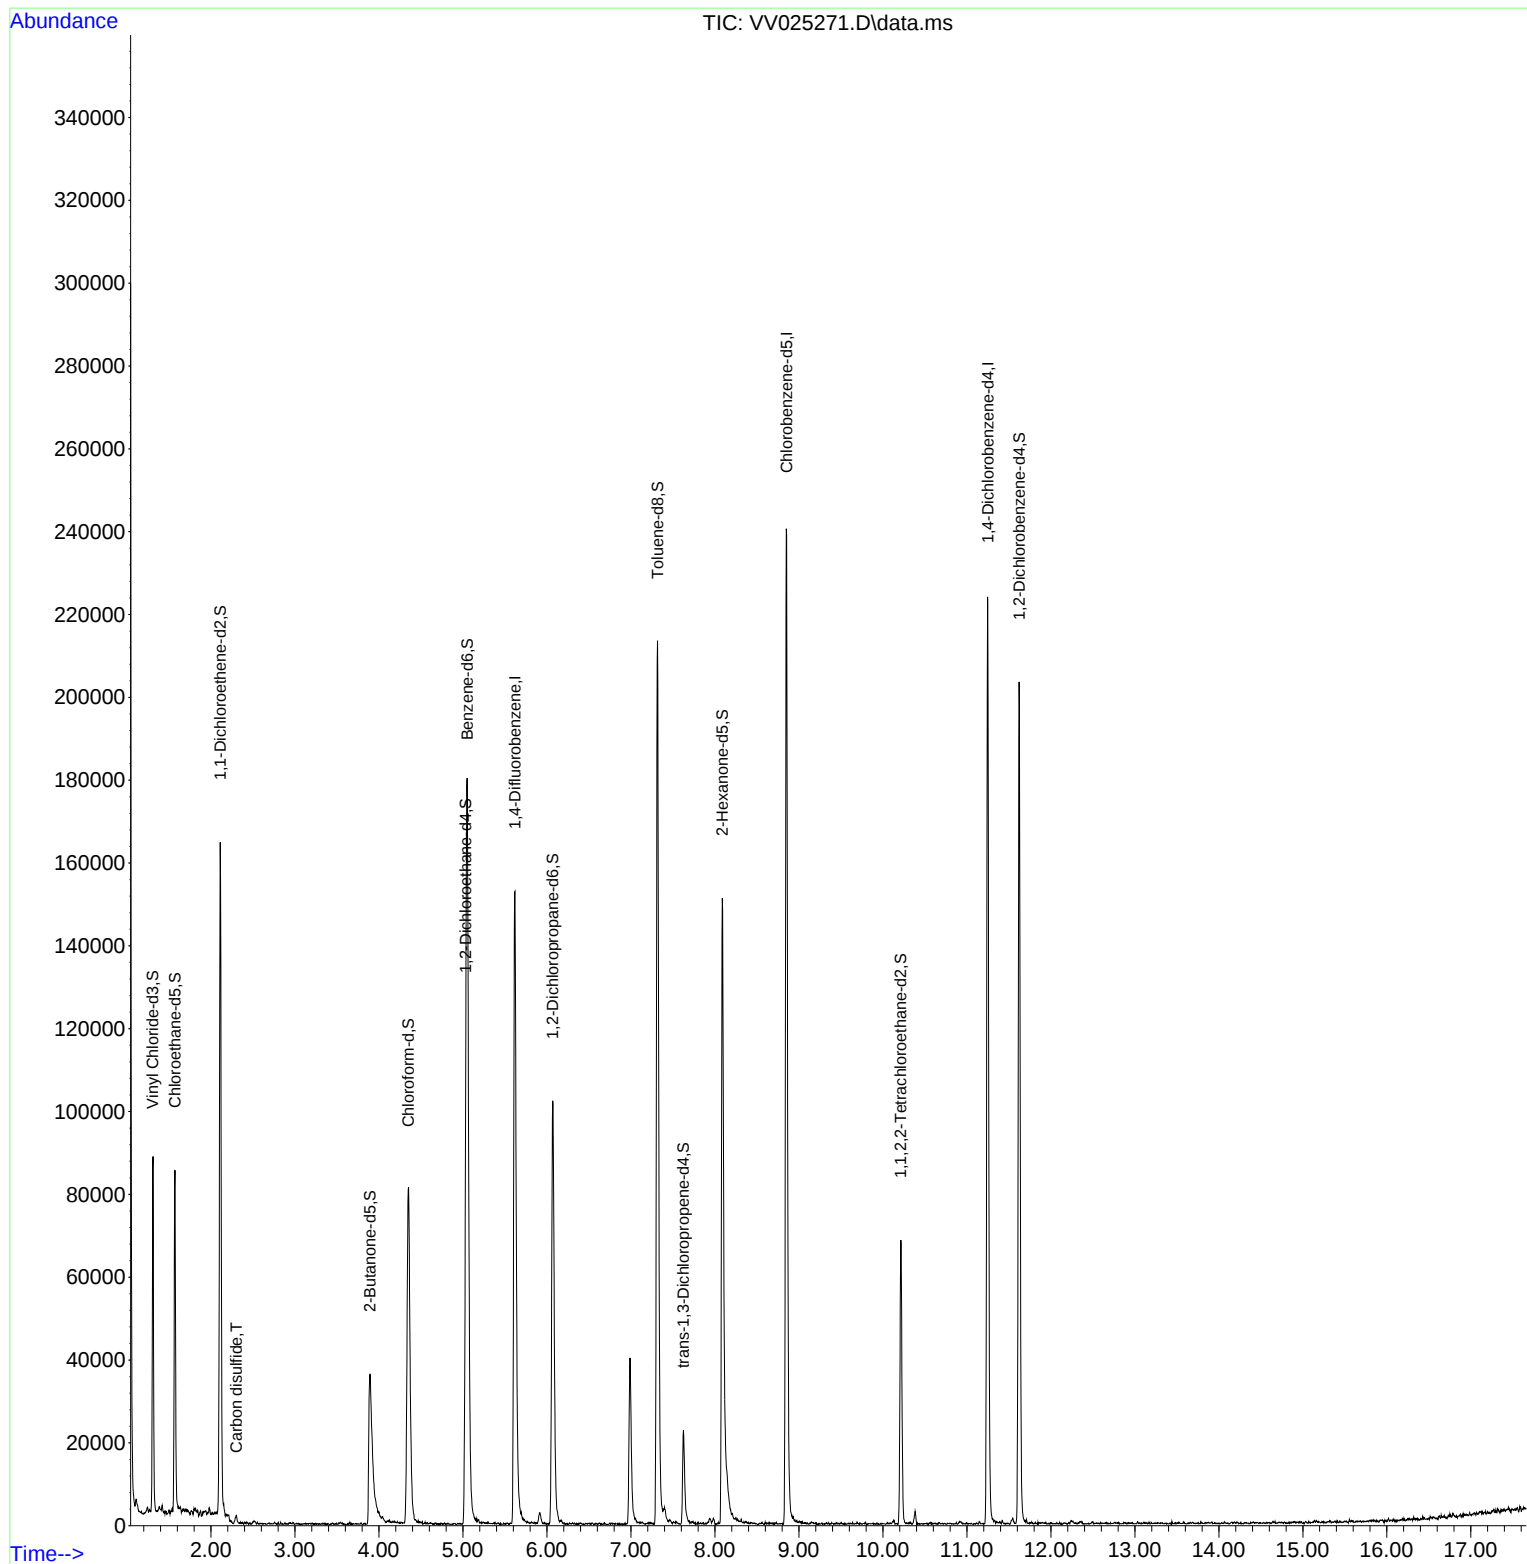

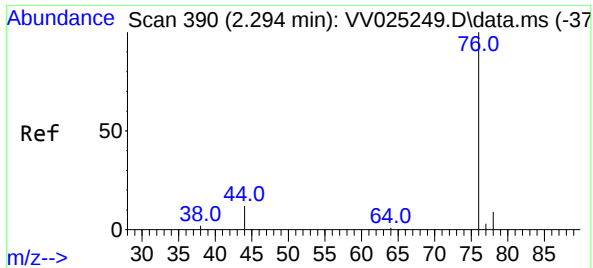

#14  
Carbon disulfide  
Concen: 0.075 ug/L  
RT: 2.301 min Scan# 391  
Delta R.T. 0.006 min  
Lab File: VV025271.D  
Acq: 28 Mar 2022 19:04

Instrument :  
MSVOA\_V  
ClientSampleId :  
YAZ52

Tgt Ion: 76 Resp: 2204  
Ion Ratio Lower Upper  
76 100  
78 9.6 7.0 10.4

