

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032822\
 Data File : VW025280.D
 Acq On : 28 Mar 2022 22:58
 Operator : SY/MD
 Sample : N2101-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAZ40

Quant Time: Mar 29 05:16:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 29 04:58:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	145941	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	145516	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	61997	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	46568	3.416	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	68.400%	
7) Chloroethane-d5	1.571	69	49512	4.327	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.600%	
11) 1,1-Dichloroethene-d2	2.111	63	75041	2.541	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	50.800%#	
20) 2-Butanone-d5	3.889	46	65751	48.420	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	96.840%	
24) Chloroform-d	4.349	84	80985	4.552	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.000%	
26) 1,2-Dichloroethane-d4	5.034	65	37513	4.771	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.400%	
32) Benzene-d6	5.050	84	155260	4.217	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.400%	
36) 1,2-Dichloropropane-d6	6.069	67	48176	4.669	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.400%	
41) Toluene-d8	7.317	98	134987	3.998	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.000%	
43) trans-1,3-Dichloroprop...	7.629	79	12836	3.814	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.200%	
46) 2-Hexanone-d5	8.088	63	52579	43.253	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	86.500%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32167	4.676	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	46718	4.692	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	93.800%	
Target Compounds						Qvalue
14) Carbon disulfide	2.298	76	2878	0.095	ug/L	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025280.D
Acq On : 28 Mar 2022 22:58
Operator : SY/MD
Sample : N2101-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ40


Quant Time: Mar 29 05:16:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 29 04:58:30 2022
Response via : Initial Calibration

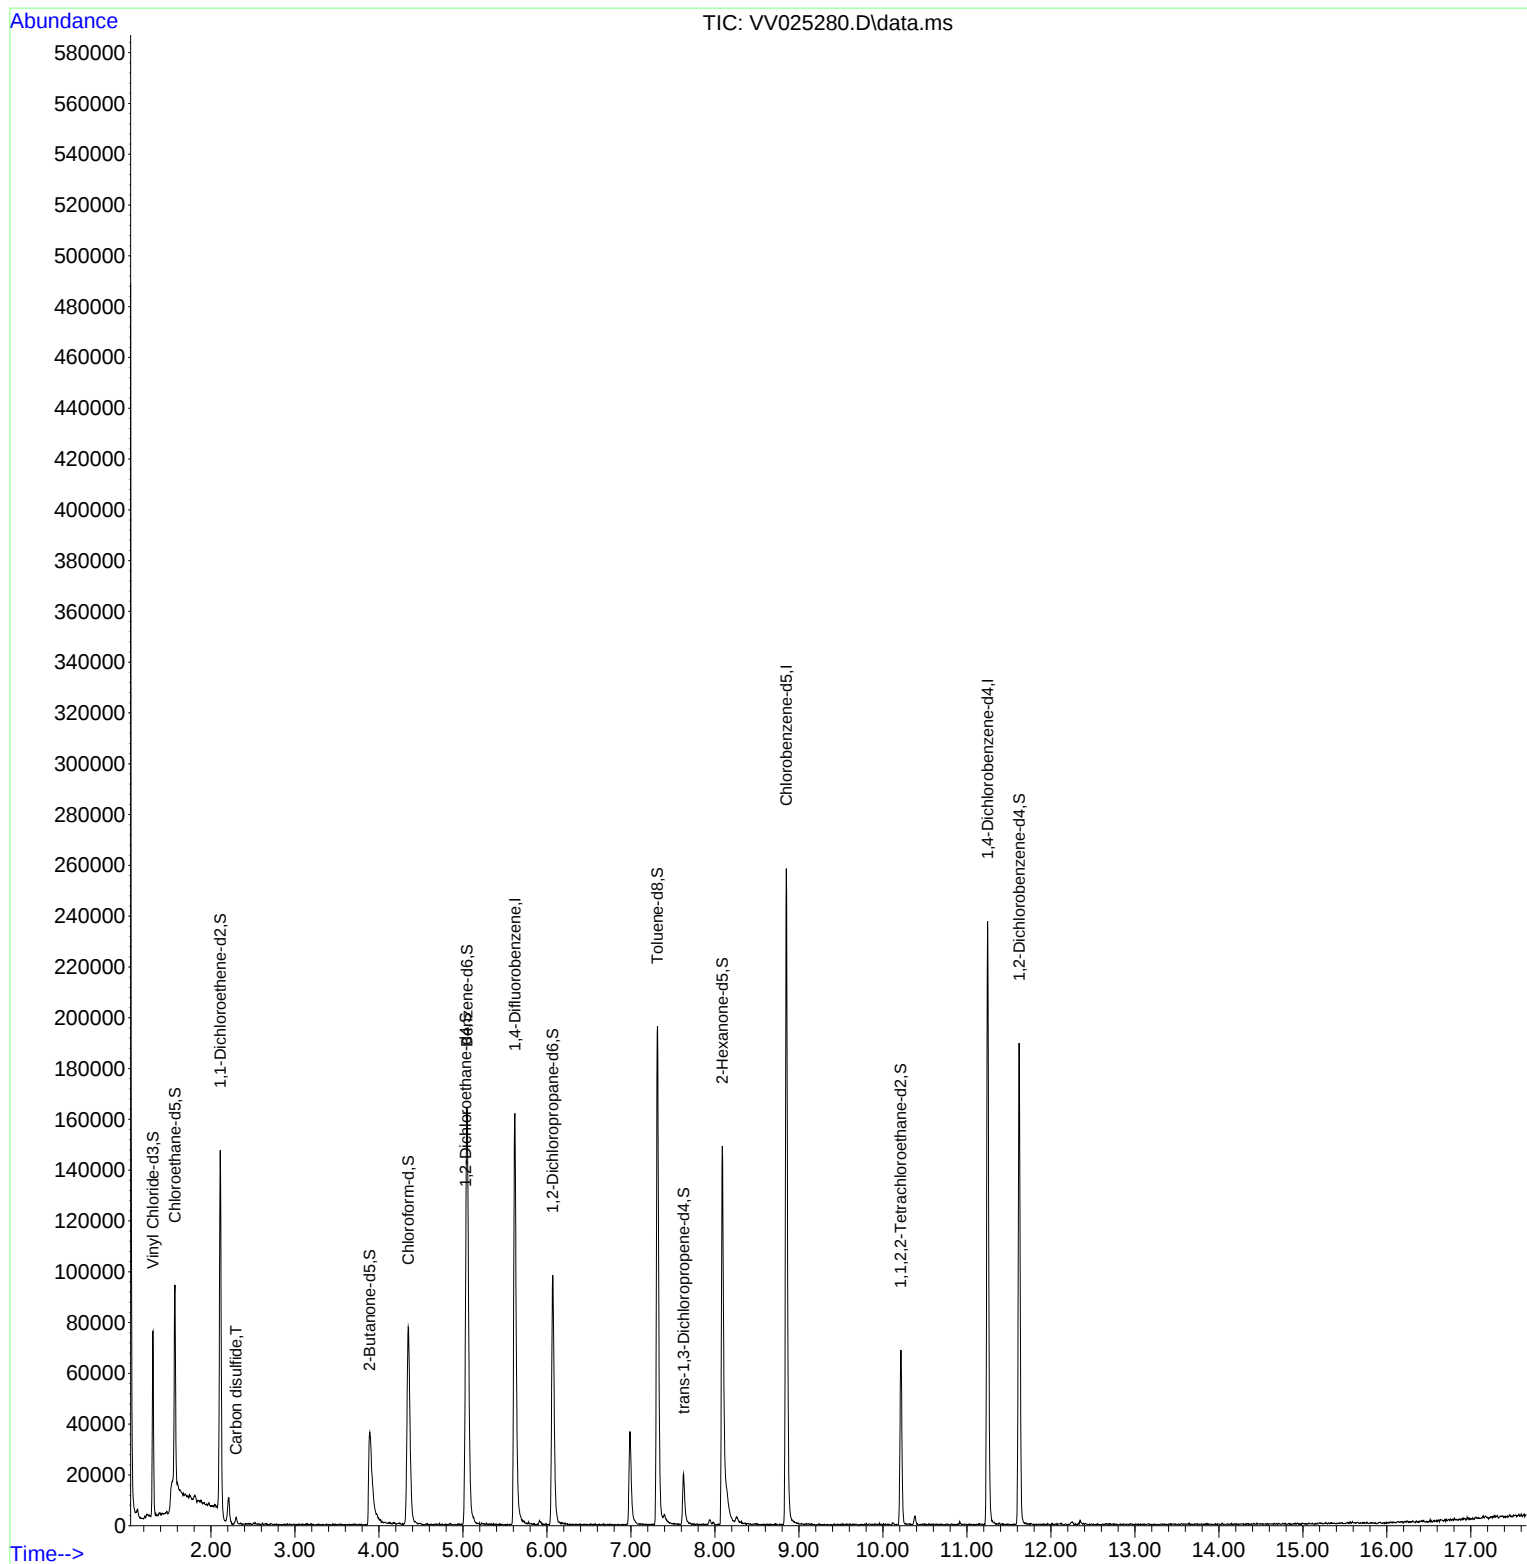

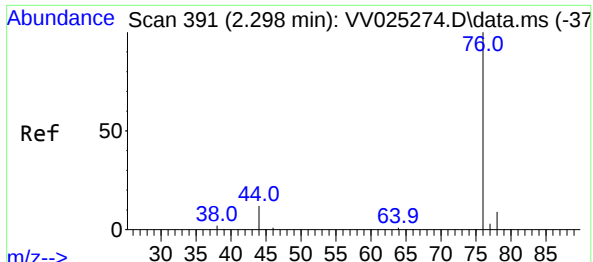

#14
Carbon disulfide
Concen: 0.095 ug/L
RT: 2.298 min Scan# 391
Delta R.T. 0.000 min
Lab File: VV025280.D
Acq: 28 Mar 2022 22:58

Instrument :
MSVOA_V
ClientSampleId :
YAZ40

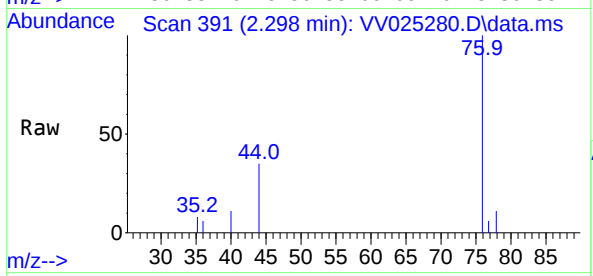

Tgt Ion: 76 Resp: 2878
Ion Ratio Lower Upper
76 100
78 11.0 7.0 10.4#

