

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025250.D
 Acq On : 28 Mar 2022 10:44
 Operator : SY/MD
 Sample : VV0328WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	47	62	64	rBV7	5800	9477	1.93%	0.234%
2	1.307	76	83	97	rVB	106216	109562	22.30%	2.703%
3	1.568	156	164	176	rVB	94824	106924	21.76%	2.638%
4	2.105	321	331	354	rVB	216778	322360	65.60%	7.954%
5	2.507	448	456	465	rBV5	2993	5028	1.02%	0.124%
6	3.918	883	895	904	rBV2	17954	48719	9.91%	1.202%
7	4.346	1011	1028	1059	rVB	85662	220564	44.89%	5.442%
8	5.043	1229	1245	1279	rBV2	195319	491394	100.00%	12.125%
9	5.613	1409	1422	1445	rBV	170333	349677	71.16%	8.628%
10	6.066	1548	1563	1583	rBV	107929	227640	46.33%	5.617%
11	6.982	1836	1848	1872	rBV	44902	89982	18.31%	2.220%
12	7.310	1939	1950	1968	rBV	231643	416068	84.67%	10.266%
13	7.622	2036	2047	2066	rBV2	25492	48438	9.86%	1.195%
14	7.976	2148	2157	2167	rBV6	4339	6703	1.36%	0.165%
15	8.088	2182	2192	2225	rBV	143504	332524	67.67%	8.205%
16	8.847	2418	2428	2458	rBV	256283	431563	87.82%	10.648%
17	10.214	2842	2853	2868	rBV	74152	118675	24.15%	2.928%
18	11.246	3164	3174	3194	rBV	240759	375032	76.32%	9.254%
19	11.622	3280	3291	3310	rBV	211130	336605	68.50%	8.305%
20	13.014	3720	3724	3728	rBV	8285	5923	1.21%	0.146%




Sum of corrected areas: 4052858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025250.D
Acq On : 28 Mar 2022 10:44
Operator : SY/MD
Sample : VV0328WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

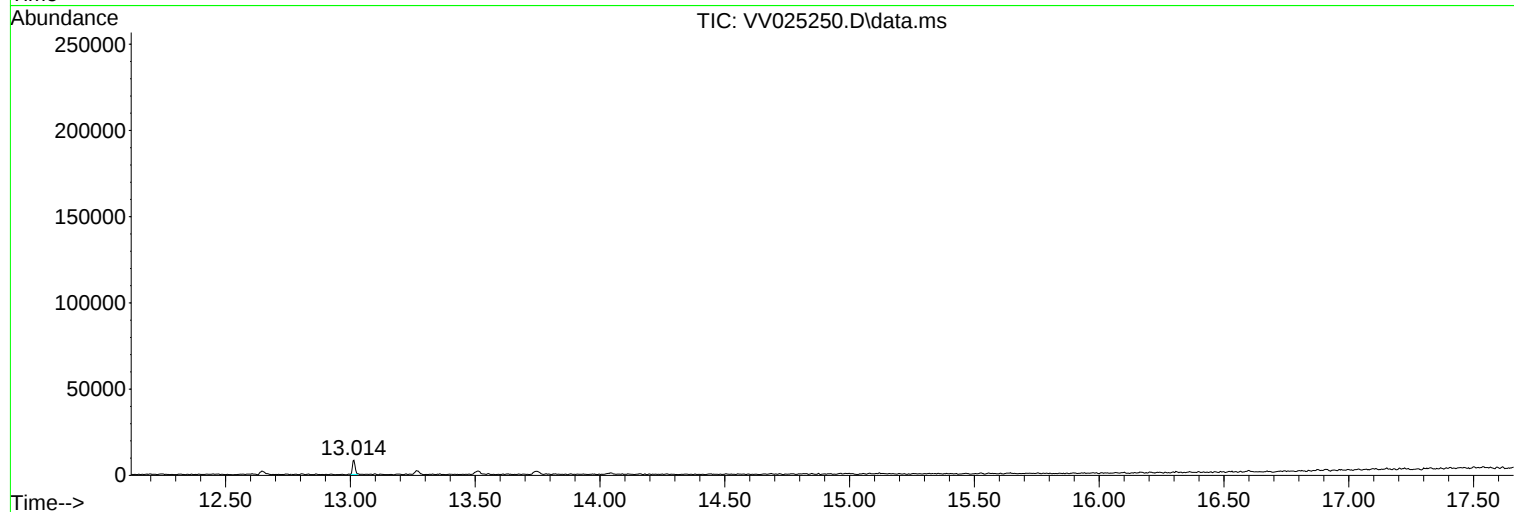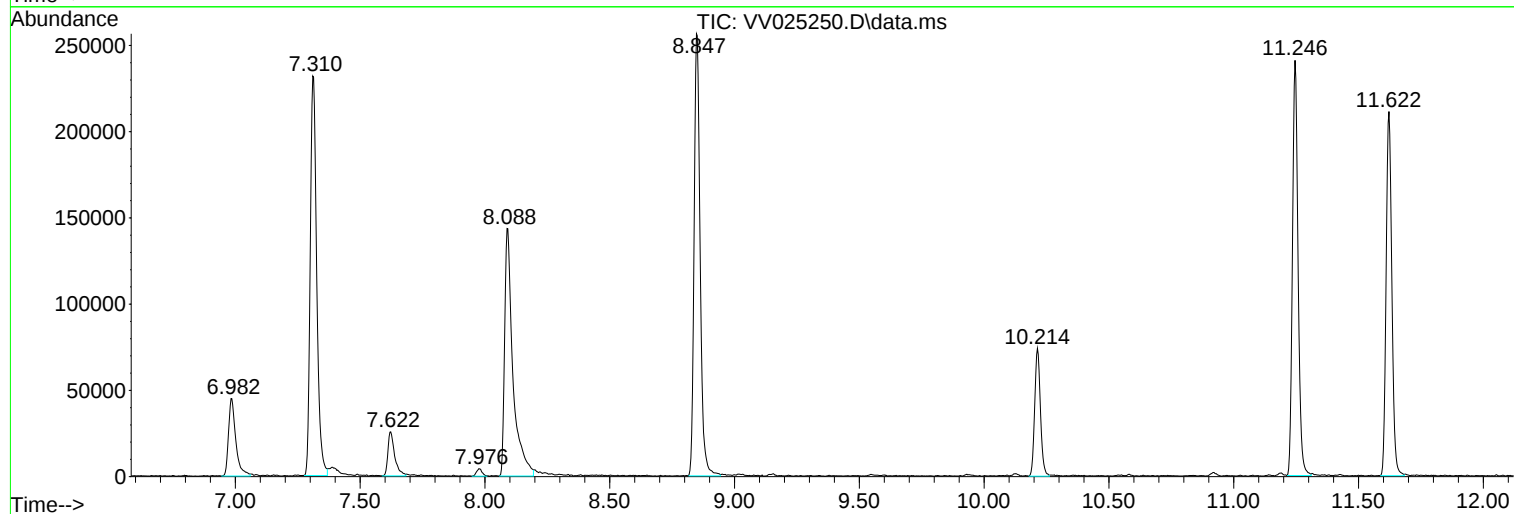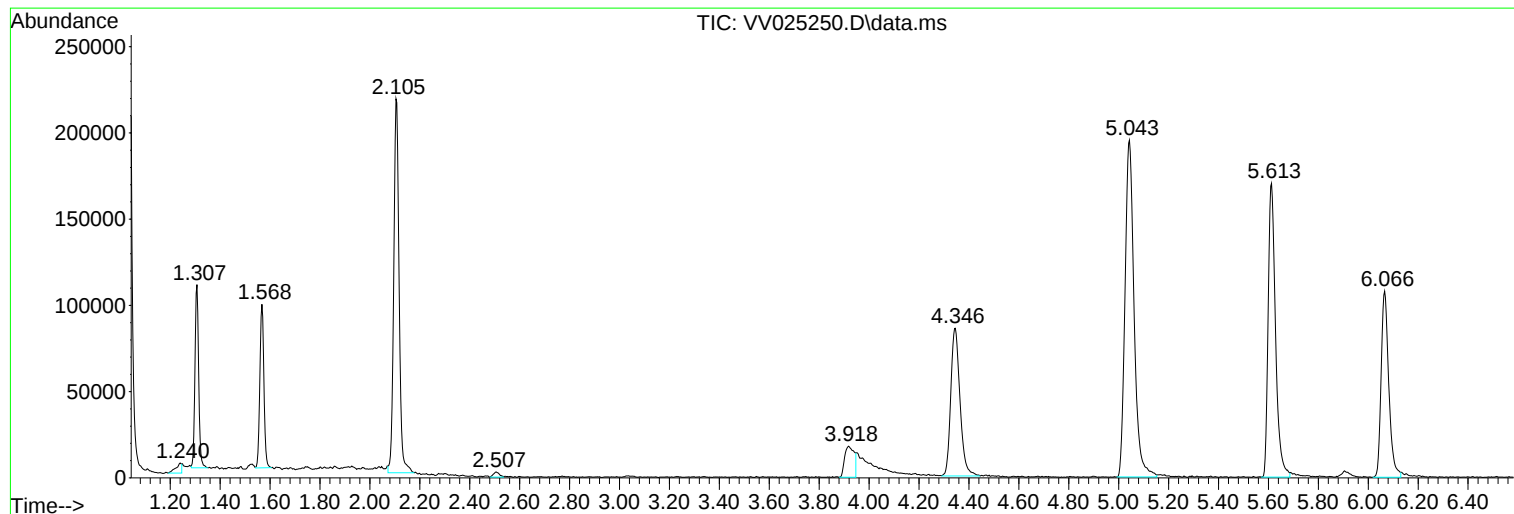

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025250.D
Acq On : 28 Mar 2022 10:44
Operator : SY/MD
Sample : VV0328WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025250.D
Acq On : 28 Mar 2022 10:44
Operator : SY/MD
Sample : VV0328WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------