

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025256.D
 Acq On : 28 Mar 2022 13:14
 Operator : SY/MD
 Sample : N2110-01DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	104159	104037	21.99%	2.438%
2	1.568	156	164	180	rVB	91504	106066	22.41%	2.485%
3	2.108	321	332	357	rVB	200532	299785	63.35%	7.024%
4	3.924	887	897	898	rBV	17936	24691	5.22%	0.579%
5	4.352	1012	1030	1059	rBV	83523	214804	45.39%	5.033%
6	5.047	1228	1246	1274	rBV2	187956	473213	100.00%	11.088%
7	5.616	1410	1423	1452	rBV	174083	363232	76.76%	8.511%
8	5.908	1506	1514	1527	rBV8	3900	8453	1.79%	0.198%
9	6.069	1551	1564	1584	rBV	105912	219495	46.38%	5.143%
10	6.989	1839	1850	1874	rBV	43262	84199	17.79%	1.973%
11	7.317	1941	1952	1971	rBV	220027	395418	83.56%	9.265%
12	7.391	1972	1975	1990	rVB7	3536	6962	1.47%	0.163%
13	7.625	2039	2048	2063	rBV2	23999	43686	9.23%	1.024%
14	7.976	2140	2157	2176	rBV	183706	312246	65.98%	7.316%
15	8.091	2183	2193	2232	rBV	142920	332087	70.18%	7.781%
16	8.850	2417	2429	2454	rBV	271913	448808	94.84%	10.516%
17	10.214	2842	2853	2873	rBV	70665	113594	24.00%	2.662%
18	11.246	3163	3174	3204	rBV	246943	390262	82.47%	9.144%
19	11.622	3279	3291	3311	rBV	203943	326853	69.07%	7.658%




Sum of corrected areas: 4267891

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025256.D
Acq On : 28 Mar 2022 13:14
Operator : SY/MD
Sample : N2110-01DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

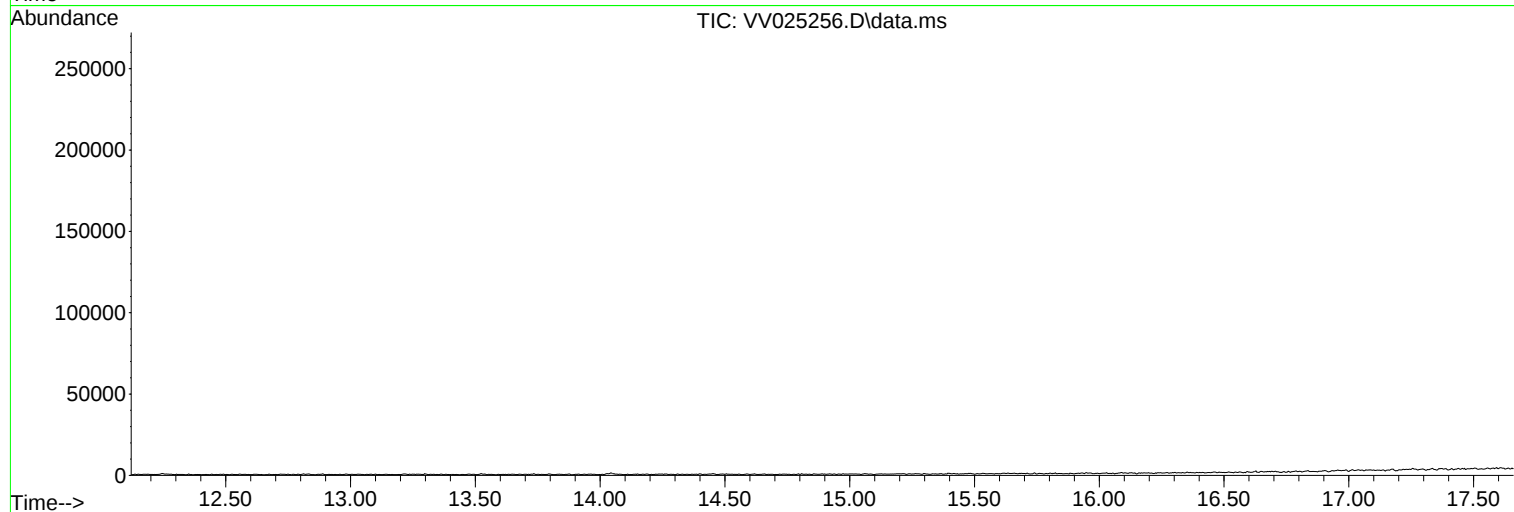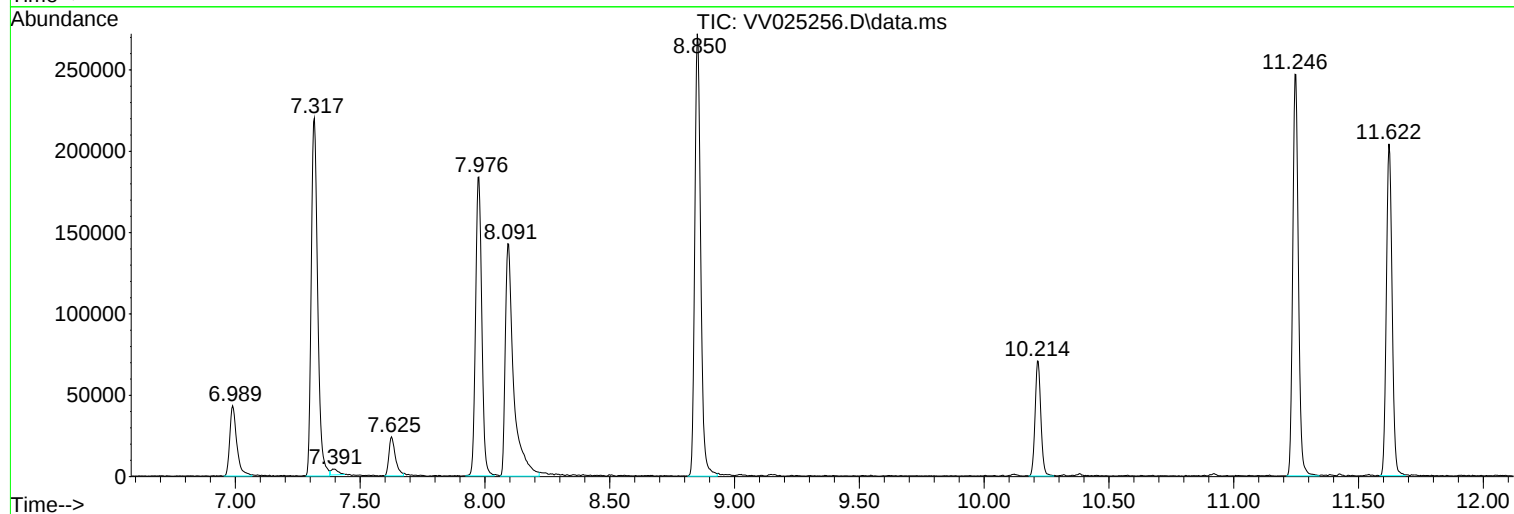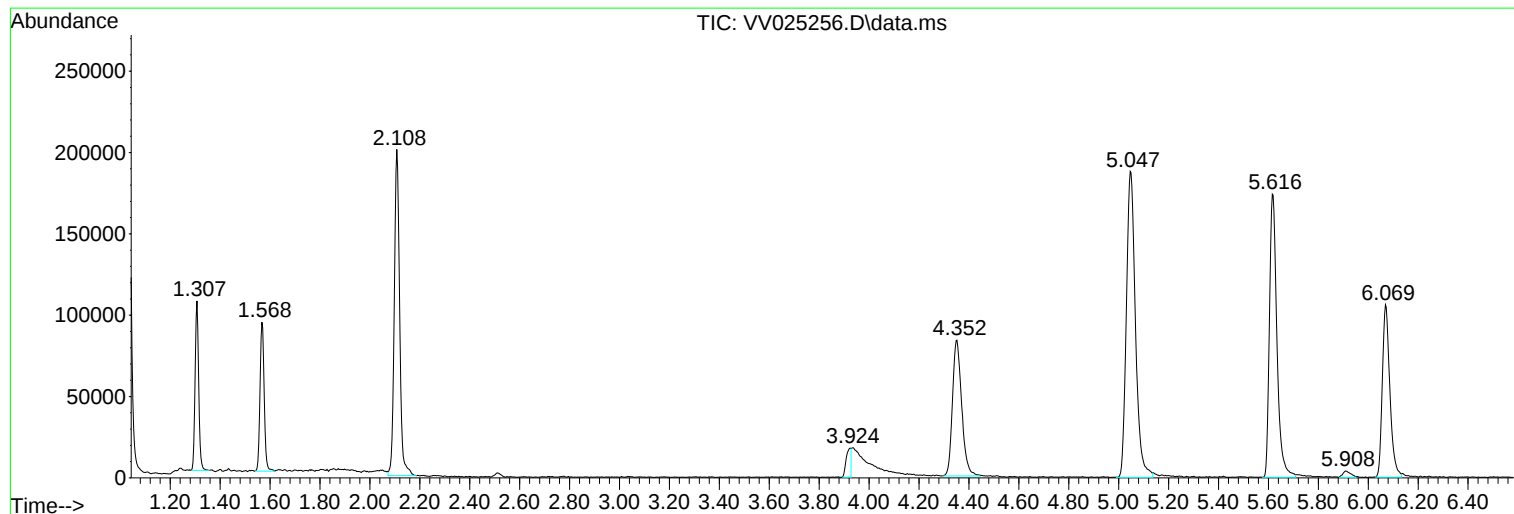

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025256.D
Acq On : 28 Mar 2022 13:14
Operator : SY/MD
Sample : N2110-01DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025256.D
Acq On : 28 Mar 2022 13:14
Operator : SY/MD
Sample : N2110-01DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc