

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025258.D
 Acq On : 28 Mar 2022 14:01
 Operator : SY/MD
 Sample : N2110-03DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	100433	99727	22.32%	2.533%
2	1.568	156	164	177	rBV	89312	101326	22.68%	2.573%
3	2.108	322	332	359	rVB	189655	284440	63.67%	7.223%
4	3.918	886	895	897	rBV2	16277	20290	4.54%	0.515%
5	4.349	1012	1029	1056	rBV	80223	204107	45.69%	5.183%
6	5.047	1231	1246	1272	rBV2	178386	446737	100.00%	11.345%
7	5.619	1412	1424	1444	rBV	152285	318276	71.24%	8.083%
8	5.918	1506	1517	1520	rBV5	3652	5867	1.31%	0.149%
9	6.069	1551	1564	1588	rBV	99465	208944	46.77%	5.306%
10	6.989	1840	1850	1869	rBV2	39620	78605	17.60%	1.996%
11	7.317	1940	1952	1974	rBV	216701	380550	85.18%	9.664%
12	7.625	2036	2048	2062	rBV3	22675	42420	9.50%	1.077%
13	7.976	2145	2157	2172	rBV2	162797	277774	62.18%	7.054%
14	8.092	2184	2193	2237	rBV	133121	308851	69.13%	7.843%
15	8.850	2419	2429	2446	rBV	243285	398781	89.27%	10.127%
16	10.217	2840	2854	2867	rBV	66664	107535	24.07%	2.731%
17	11.246	3163	3174	3196	rBV	215591	342503	76.67%	8.698%
18	11.622	3278	3291	3309	rBV	192032	311004	69.62%	7.898%




Sum of corrected areas: 3937737

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025258.D
Acq On : 28 Mar 2022 14:01
Operator : SY/MD
Sample : N2110-03DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

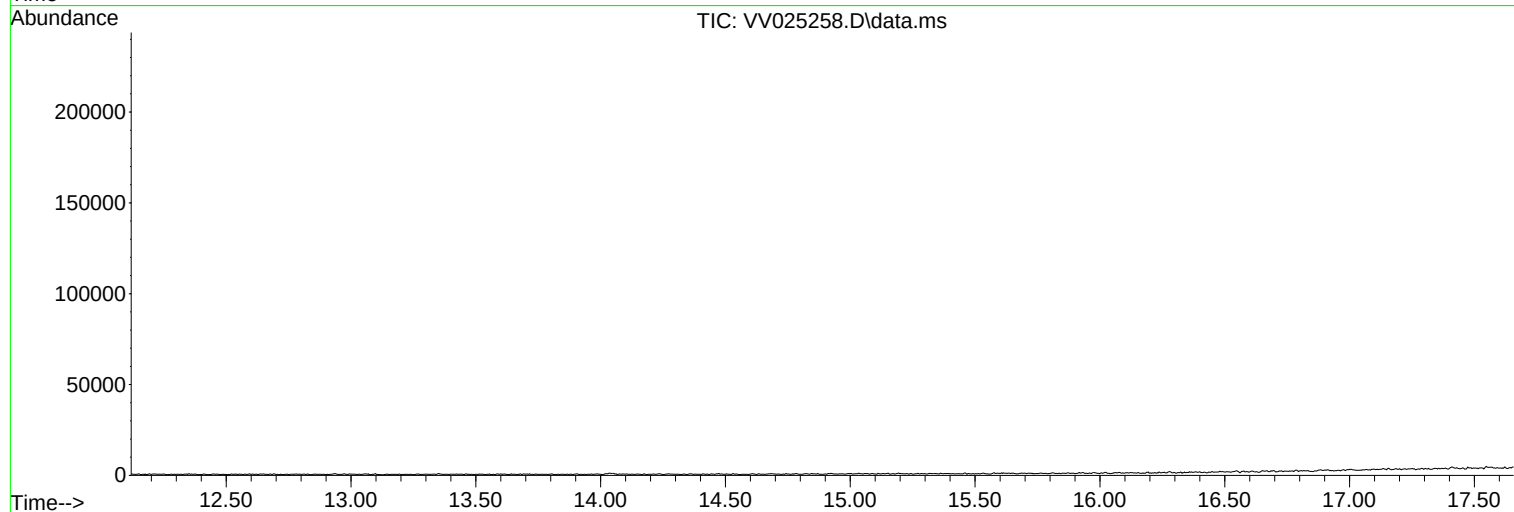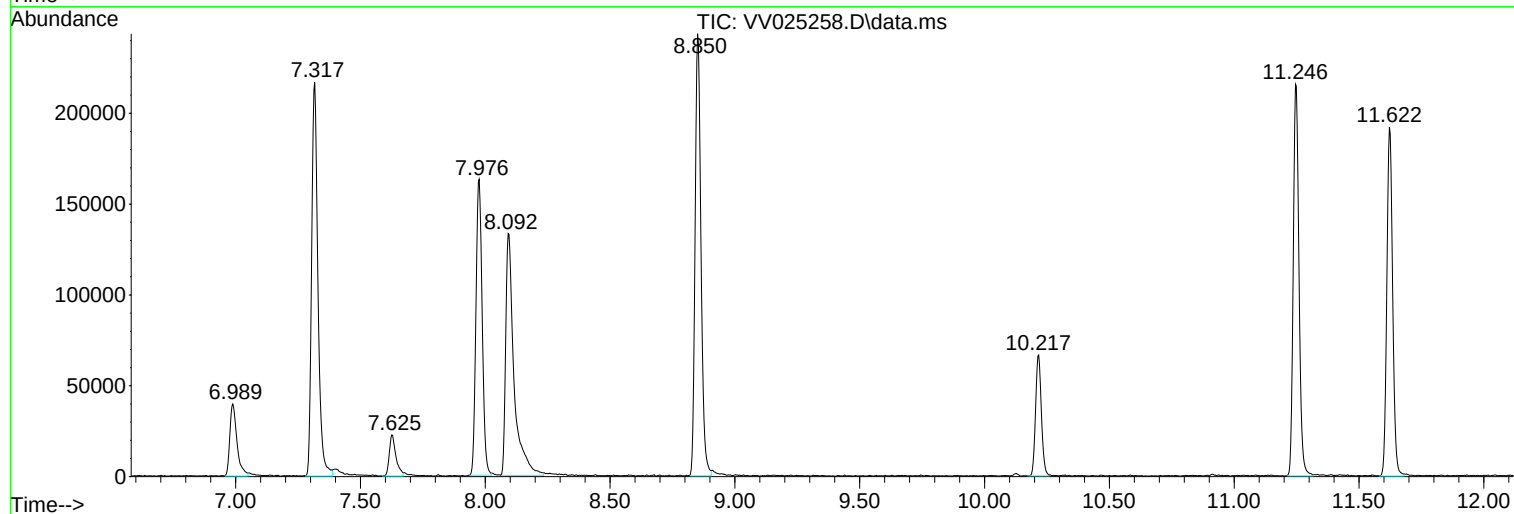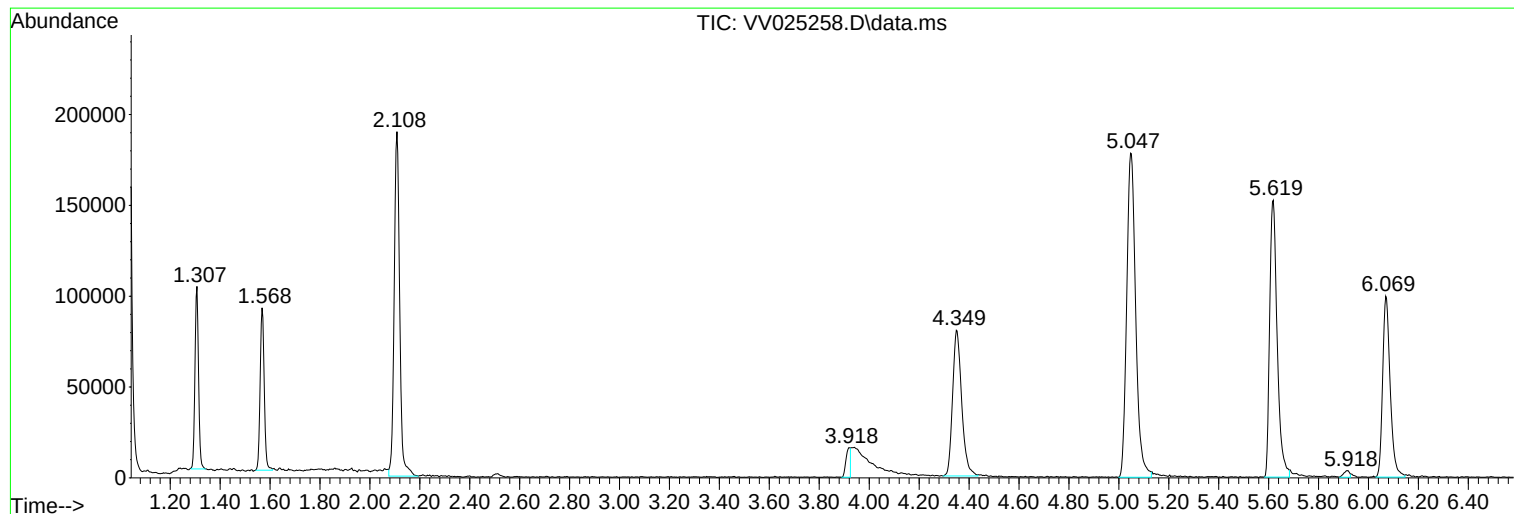

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025258.D
Acq On : 28 Mar 2022 14:01
Operator : SY/MD
Sample : N2110-03DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025258.D
Acq On : 28 Mar 2022 14:01
Operator : SY/MD
Sample : N2110-03DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc