

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025259.D
 Acq On : 28 Mar 2022 14:24
 Operator : SY/MD
 Sample : N2110-06DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PB6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	100634	103496	23.00%	2.615%
2	1.568	157	164	176	rBV	88389	100307	22.30%	2.535%
3	2.108	322	332	355	rVB	187286	282011	62.68%	7.126%
4	3.924	886	897	909	rBV	17418	53947	11.99%	1.363%
5	4.349	1014	1029	1054	rBV	79045	202640	45.04%	5.120%
6	5.050	1230	1247	1283	rBV2	178133	449891	100.00%	11.368%
7	5.616	1412	1423	1451	rBV	155821	329986	73.35%	8.338%
8	5.912	1507	1515	1518	rBV5	3196	4519	1.00%	0.114%
9	6.069	1550	1564	1590	rBV2	98621	212186	47.16%	5.362%
10	6.989	1836	1850	1875	rBV	41227	80907	17.98%	2.044%
11	7.317	1941	1952	1972	rBV	209634	374668	83.28%	9.467%
12	7.625	2039	2048	2063	rBV2	22383	42245	9.39%	1.067%
13	7.976	2142	2157	2172	rBV	132433	228595	50.81%	5.776%
14	8.092	2183	2193	2234	rBV	131639	305598	67.93%	7.722%
15	8.850	2415	2429	2456	rBV	246313	411803	91.53%	10.406%
16	10.217	2844	2854	2869	rBV	67856	105935	23.55%	2.677%
17	11.246	3161	3174	3199	rBV	227290	357601	79.49%	9.036%
18	11.622	3278	3291	3307	rBV	197301	311147	69.16%	7.862%




Sum of corrected areas: 3957482

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025259.D
Acq On : 28 Mar 2022 14:24
Operator : SY/MD
Sample : N2110-06DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

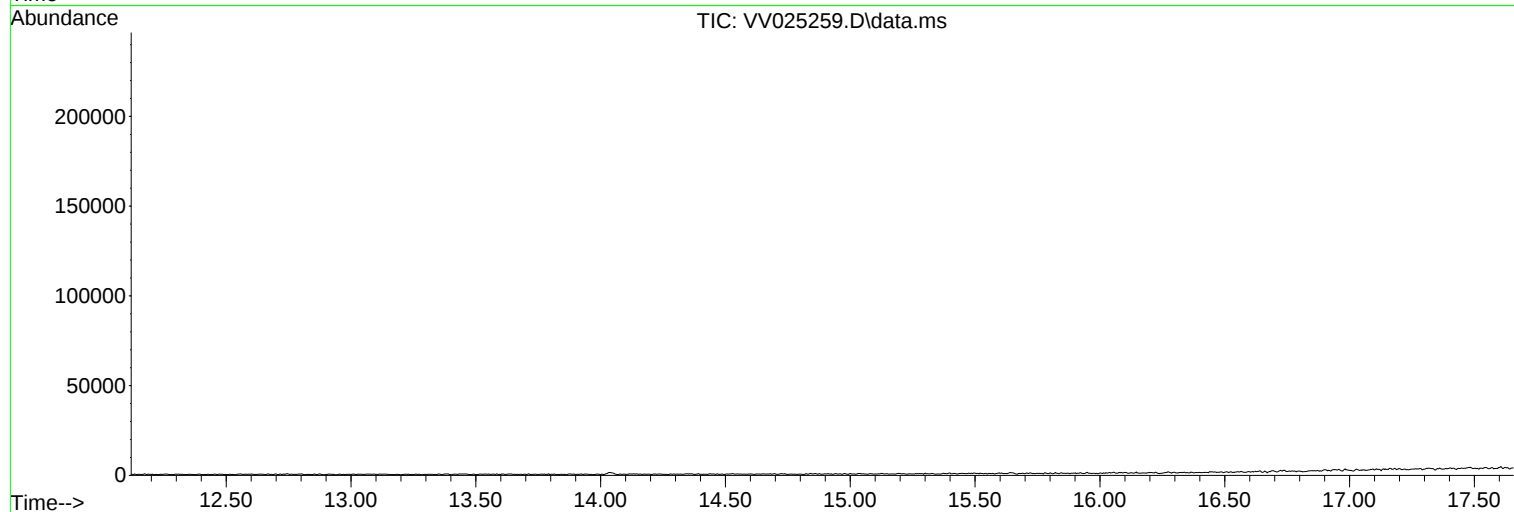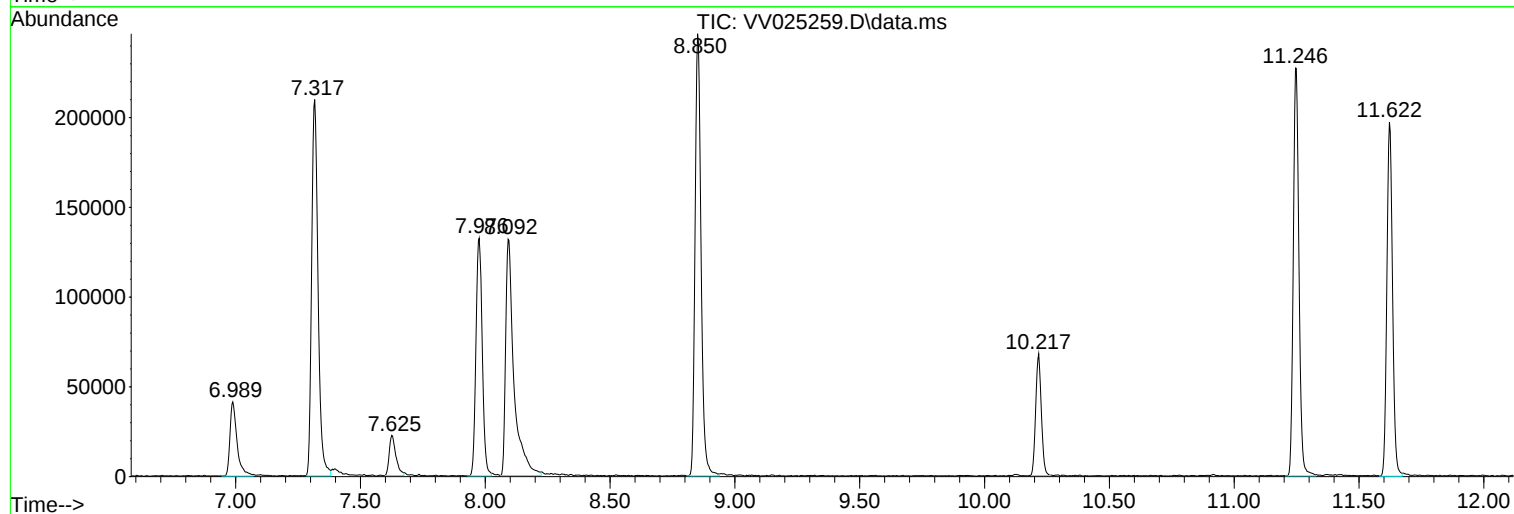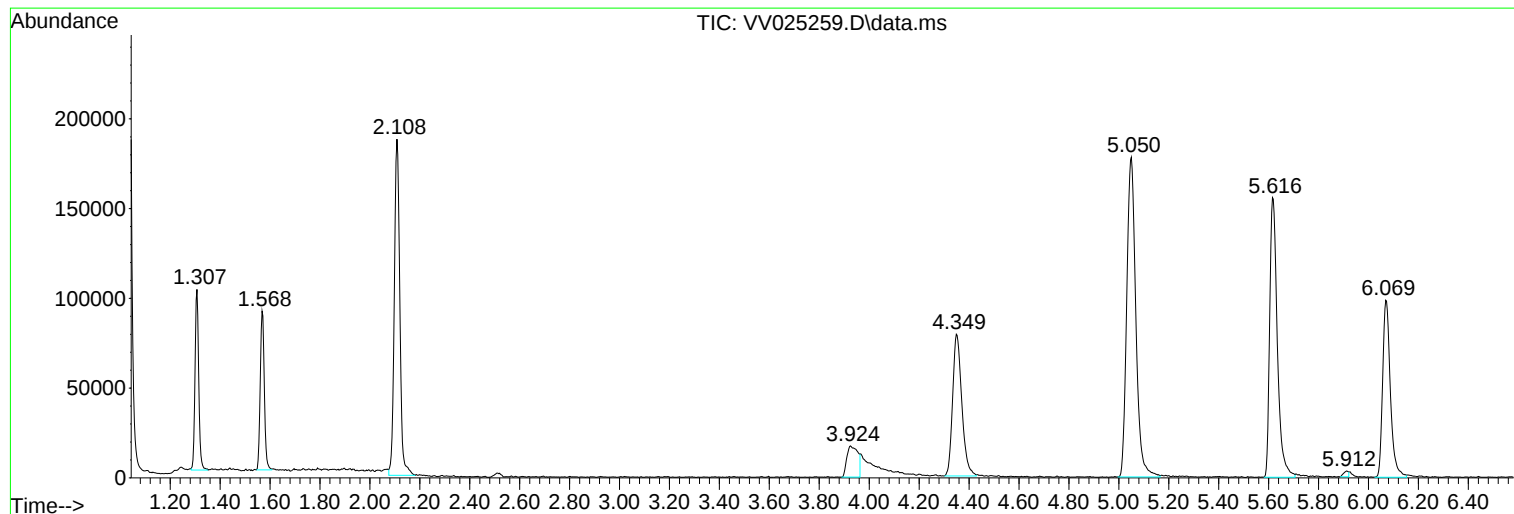

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025259.D
Acq On : 28 Mar 2022 14:24
Operator : SY/MD
Sample : N2110-06DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025259.D
Acq On : 28 Mar 2022 14:24
Operator : SY/MD
Sample : N2110-06DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PB6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc