

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025261.D
 Acq On : 28 Mar 2022 15:11
 Operator : SY/MD
 Sample : N2110-08DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PC0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	100376	101798	21.49%	2.411%
2	1.568	157	164	175	rBV	89000	99337	20.97%	2.352%
3	2.108	319	332	355	rVB	187339	288994	61.01%	6.843%
4	3.921	884	896	936	rBV2	21438	110523	23.33%	2.617%
5	4.352	1013	1030	1053	rBV	84928	214522	45.29%	5.080%
6	5.046	1229	1246	1278	rBV3	186842	473685	100.00%	11.217%
7	5.616	1412	1423	1448	rBV	161633	337758	71.30%	7.998%
8	5.908	1505	1514	1527	rBV10	3934	8268	1.75%	0.196%
9	6.069	1549	1564	1590	rBV2	104742	221692	46.80%	5.250%
10	6.989	1840	1850	1876	rBV2	43252	84886	17.92%	2.010%
11	7.316	1939	1952	1974	rBV	219474	395713	83.54%	9.370%
12	7.625	2038	2048	2065	rBV3	24455	45897	9.69%	1.087%
13	7.976	2143	2157	2179	rBV	154657	264768	55.90%	6.270%
14	8.091	2182	2193	2241	rBV	144117	332185	70.13%	7.866%
15	8.850	2419	2429	2450	rBV	258384	420824	88.84%	9.965%
16	10.213	2843	2853	2867	rBV	70344	112065	23.66%	2.654%
17	11.246	3163	3174	3193	rBV	245218	381993	80.64%	9.045%
18	11.622	3279	3291	3314	rBV	206520	328139	69.27%	7.770%




Sum of corrected areas: 4223047

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025261.D
Acq On : 28 Mar 2022 15:11
Operator : SY/MD
Sample : N2110-08DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

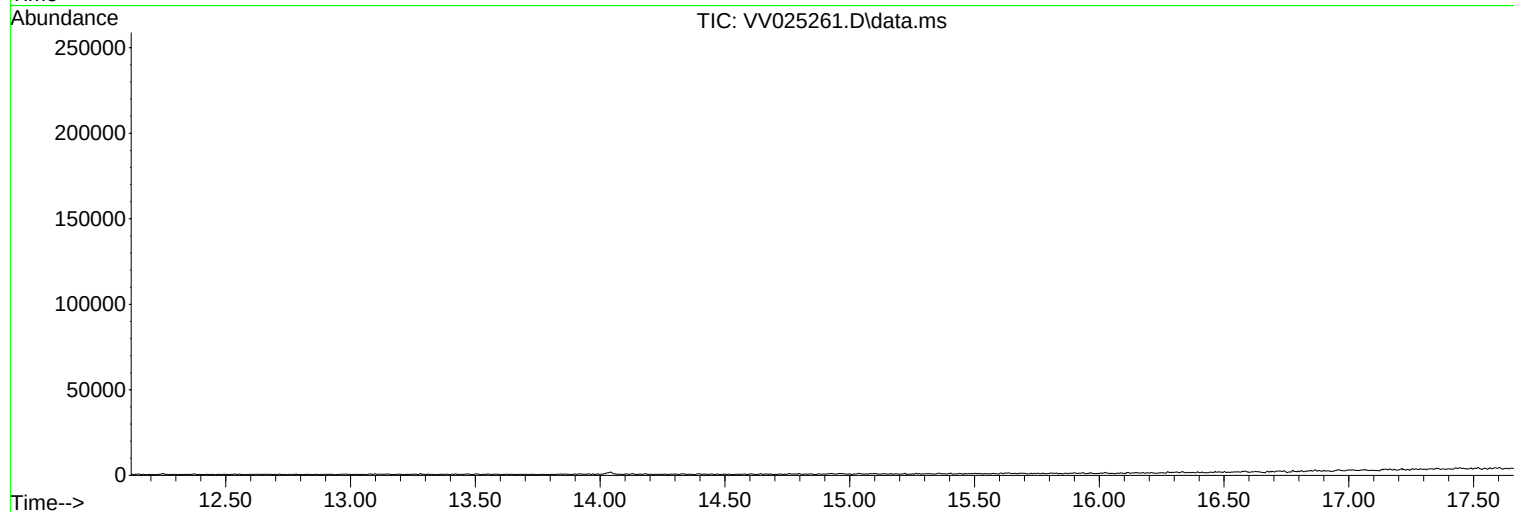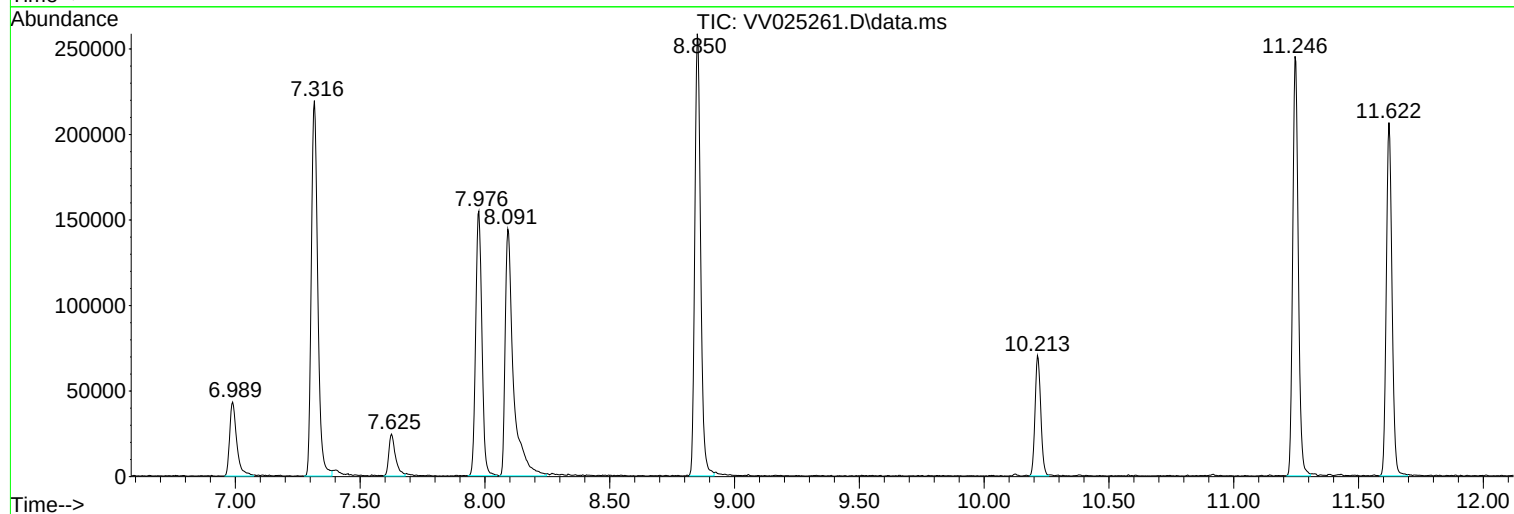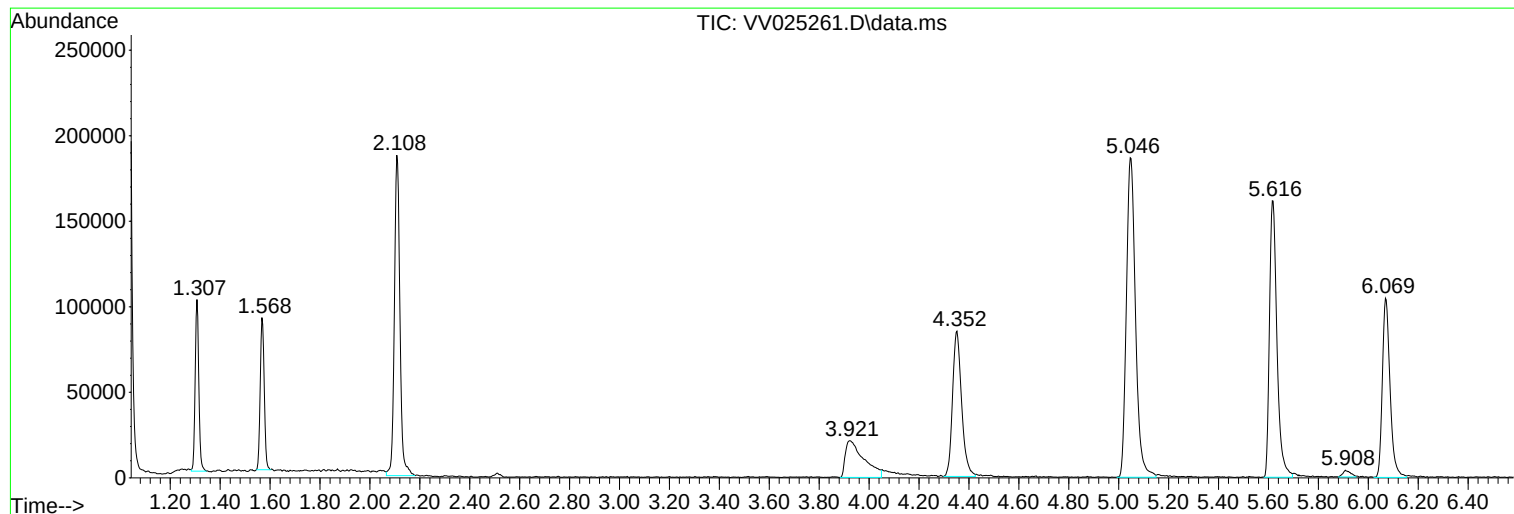

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025261.D
Acq On : 28 Mar 2022 15:11
Operator : SY/MD
Sample : N2110-08DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025261.D
Acq On : 28 Mar 2022 15:11
Operator : SY/MD
Sample : N2110-08DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc