

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025263.D
 Acq On : 28 Mar 2022 15:58
 Operator : SY/MD
 Sample : N2110-10DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PC6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	49	63	68	rBV9	3172	7282	1.18%	0.167%
2	1.307	76	83	96	rVB	99928	100785	16.32%	2.304%
3	1.568	154	164	178	rBV	88227	103340	16.73%	2.363%
4	2.108	320	332	355	rVB	190677	281632	45.61%	6.440%
5	3.928	887	898	901	rBV2	16364	30417	4.93%	0.695%
6	4.349	1011	1029	1054	rBV	80317	207328	33.57%	4.741%
7	5.047	1229	1246	1281	rBV2	183088	461927	74.80%	10.562%
8	5.619	1407	1424	1454	rBV	159131	334011	54.09%	7.637%
9	5.912	1504	1515	1526	rBV10	3519	7608	1.23%	0.174%
10	6.069	1552	1564	1587	rBV	102533	212897	34.48%	4.868%
11	6.989	1840	1850	1867	rBV	40636	78255	12.67%	1.789%
12	7.317	1941	1952	1973	rBV	214859	383919	62.17%	8.778%
13	7.625	2039	2048	2065	rBV3	21903	41713	6.76%	0.954%
14	7.973	2138	2156	2174	rBV	366132	617510	100.00%	14.119%
15	8.092	2182	2193	2236	rBV	135403	311805	50.49%	7.129%
16	8.850	2416	2429	2450	rBV	248024	409536	66.32%	9.364%
17	10.217	2840	2854	2869	rBV	67288	109101	17.67%	2.495%
18	11.246	3163	3174	3199	rBV	228844	359489	58.22%	8.220%
19	11.622	3280	3291	3308	rBV	197956	314926	51.00%	7.201%




Sum of corrected areas: 4373481

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025263.D
Acq On : 28 Mar 2022 15:58
Operator : SY/MD
Sample : N2110-10DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

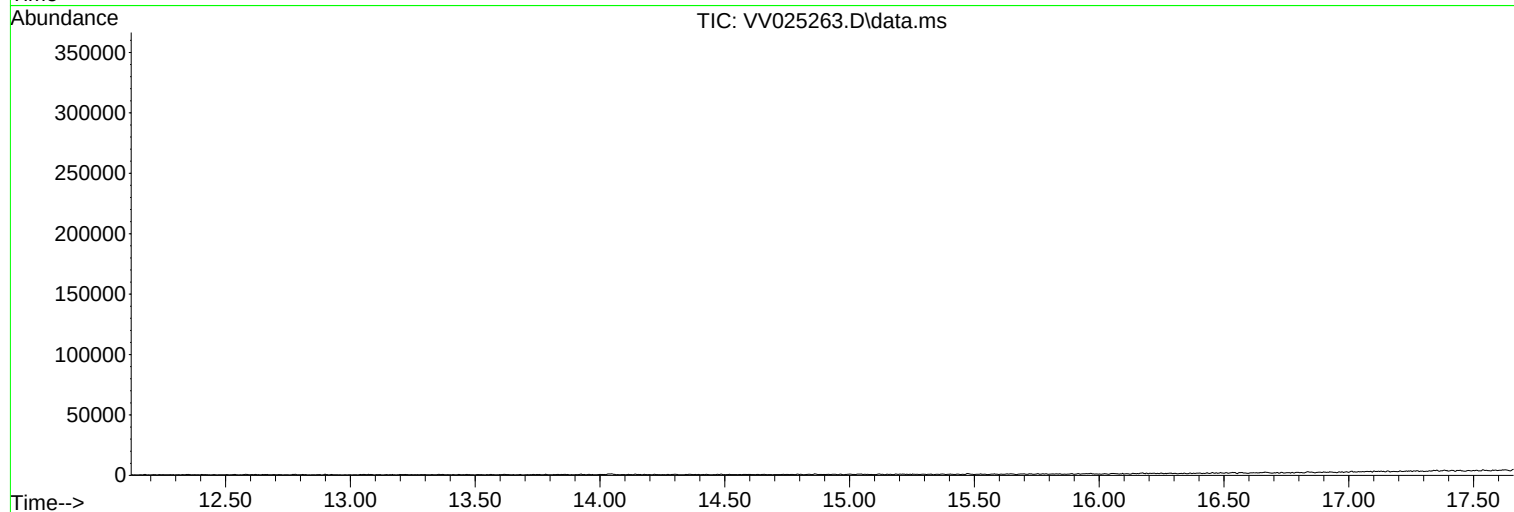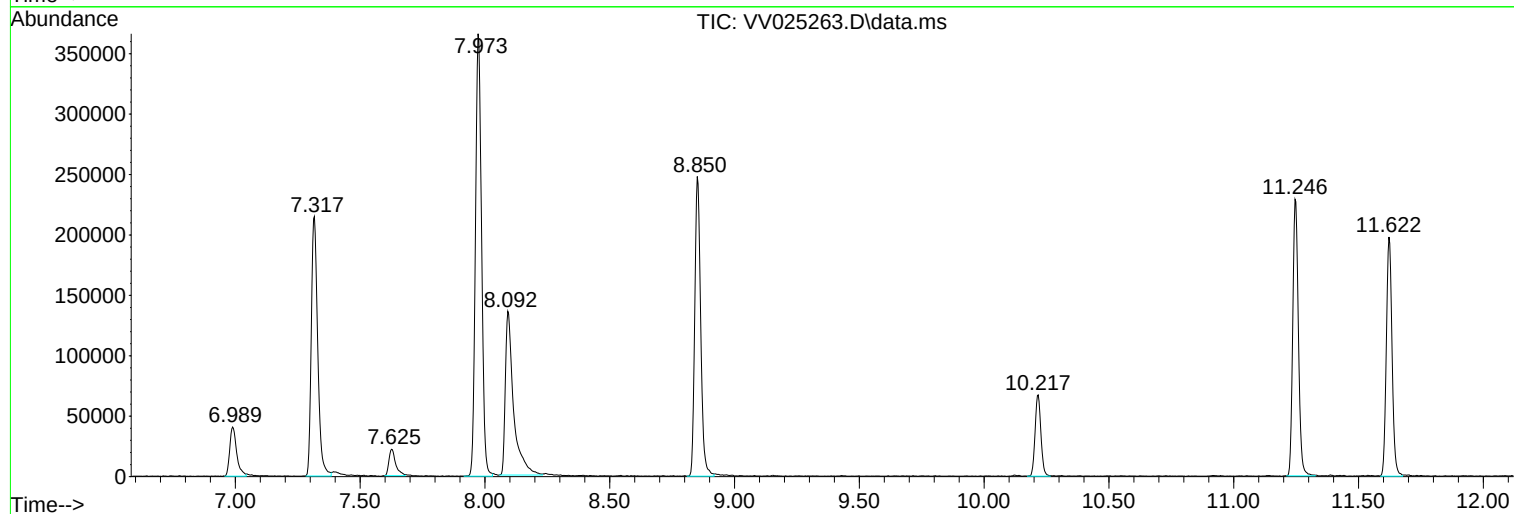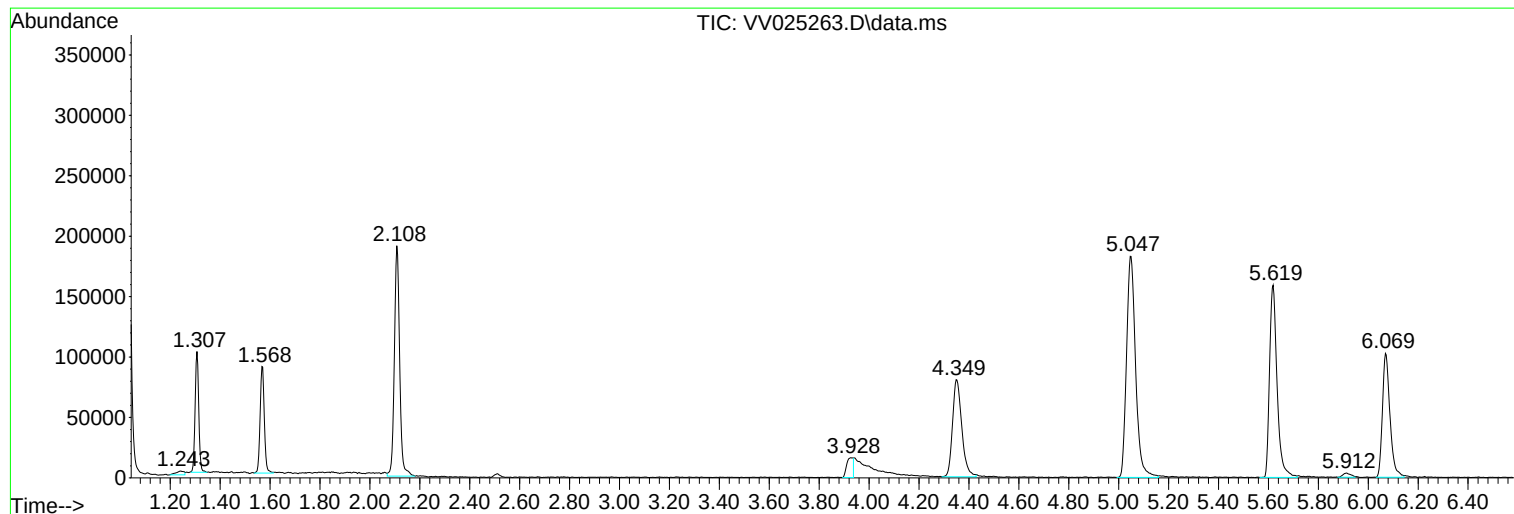

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025263.D
Acq On : 28 Mar 2022 15:58
Operator : SY/MD
Sample : N2110-10DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025263.D
Acq On : 28 Mar 2022 15:58
Operator : SY/MD
Sample : N2110-10DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc