

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025264.D
 Acq On : 28 Mar 2022 16:21
 Operator : SY/MD
 Sample : N2110-13DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0PD2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	50	63	65	rBV5	3584	5787	1.27%	0.142%
2	1.307	76	83	100	rVB	97237	99858	21.97%	2.455%
3	1.568	157	164	173	rBV	85469	94582	20.81%	2.326%
4	2.108	321	332	361	rVB	189555	288178	63.41%	7.086%
5	2.510	448	457	466	rVB5	2791	4871	1.07%	0.120%
6	3.921	885	896	900	rBV2	19534	36945	8.13%	0.908%
7	4.352	1013	1030	1058	rBV	82279	220500	48.52%	5.422%
8	5.047	1231	1246	1275	rBV2	181688	454459	100.00%	11.175%
9	5.616	1412	1423	1445	rBV	160068	331697	72.99%	8.156%
10	5.912	1506	1515	1518	rBV6	3717	5375	1.18%	0.132%
11	6.069	1551	1564	1586	rBV	101905	212972	46.86%	5.237%
12	6.989	1839	1850	1874	rBV2	40580	79781	17.56%	1.962%
13	7.317	1939	1952	1973	rBV	211703	379418	83.49%	9.330%
14	7.625	2039	2048	2062	rBV2	24001	41960	9.23%	1.032%
15	7.973	2145	2156	2183	rBV	174965	299350	65.87%	7.361%
16	8.092	2183	2193	2230	rBV	137718	311055	68.45%	7.649%
17	8.850	2419	2429	2454	rBV	255802	415354	91.40%	10.213%
18	10.217	2842	2854	2867	rBV2	68324	108224	23.81%	2.661%
19	11.246	3160	3174	3196	rBV	233227	362190	79.70%	8.906%
20	11.622	3278	3291	3307	rBV	200251	314264	69.15%	7.728%




Sum of corrected areas: 4066820

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025264.D
Acq On : 28 Mar 2022 16:21
Operator : SY/MD
Sample : N2110-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

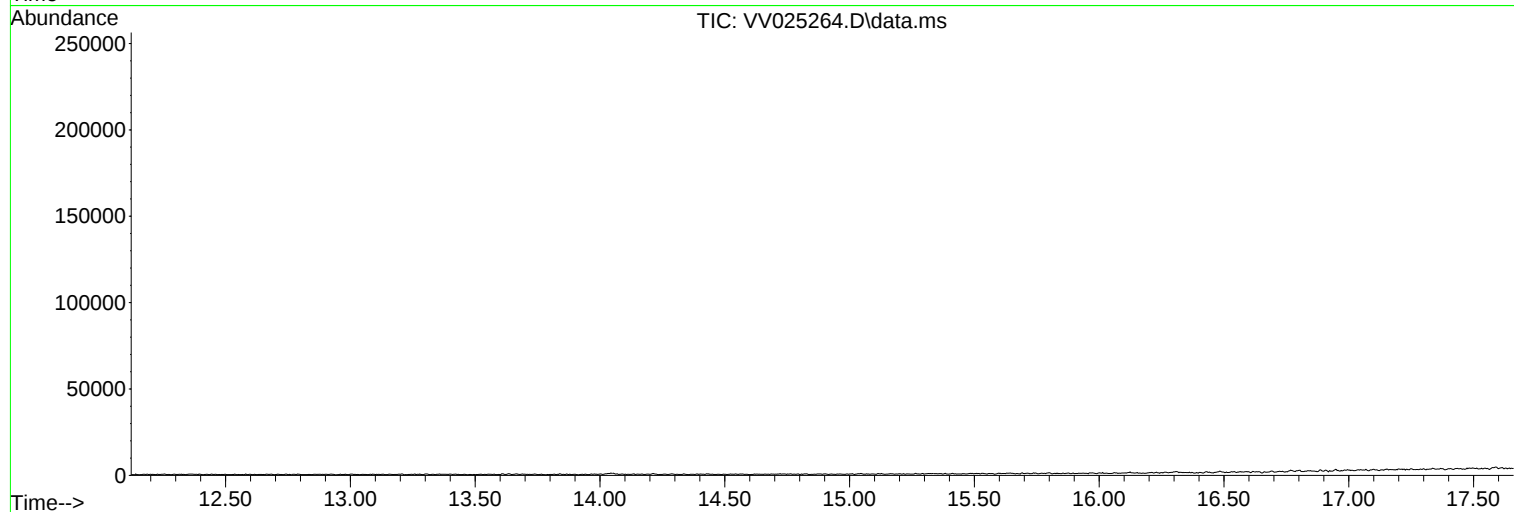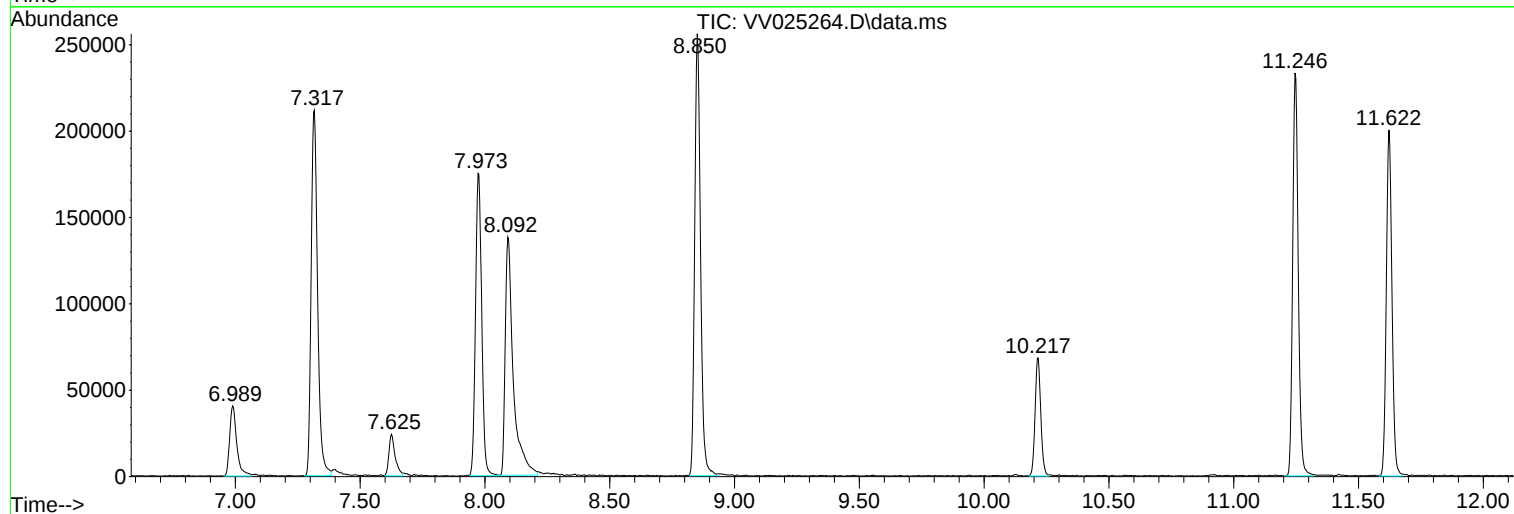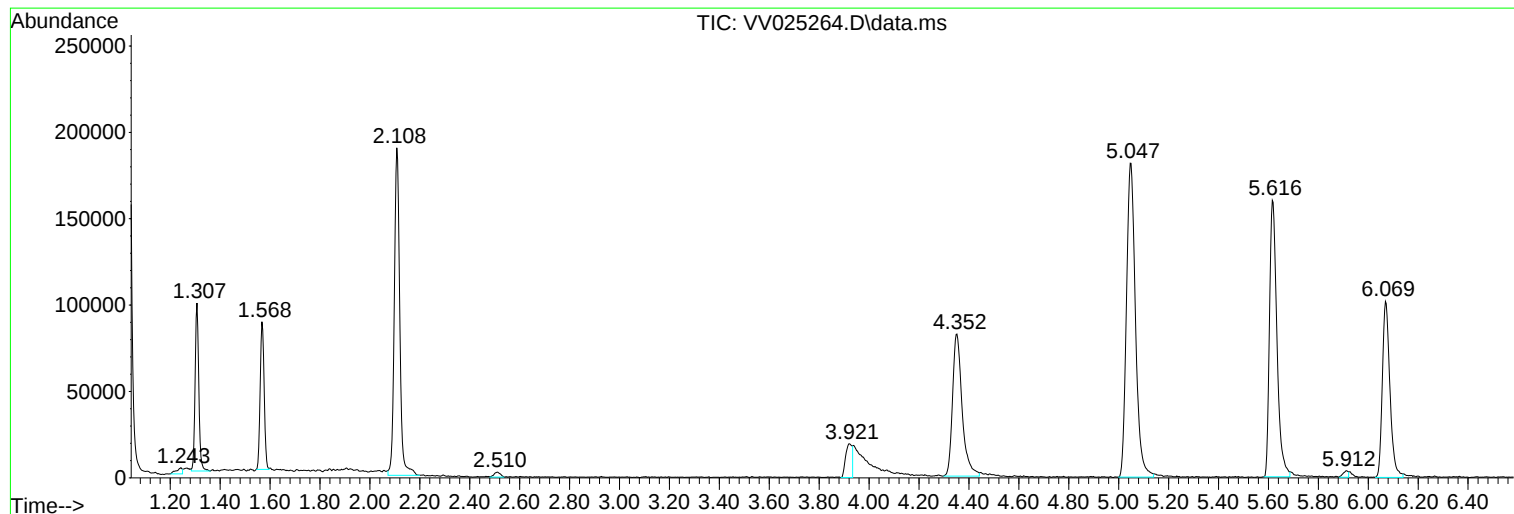

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025264.D
Acq On : 28 Mar 2022 16:21
Operator : SY/MD
Sample : N2110-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025264.D
Acq On : 28 Mar 2022 16:21
Operator : SY/MD
Sample : N2110-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0PD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc