

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025266.D
 Acq On : 28 Mar 2022 17:08
 Operator : SY/MD
 Sample : N2101-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAZ69

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025266.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rVB	98654	96471	21.56%	2.606%
2	1.568	157	164	173	rBV	86330	96797	21.63%	2.615%
3	2.108	320	332	356	rVB	181269	273681	61.15%	7.393%
4	3.921	886	896	898	rBV	20443	30936	6.91%	0.836%
5	4.349	1013	1029	1053	rBV2	79253	201420	45.01%	5.441%
6	5.047	1231	1246	1282	rBV3	177346	447531	100.00%	12.089%
7	5.619	1412	1424	1448	rBV	159475	327356	73.15%	8.843%
8	5.912	1505	1515	1517	rBV4	4456	5800	1.30%	0.157%
9	6.069	1550	1564	1589	rBV2	100349	208968	46.69%	5.645%
10	6.989	1840	1850	1870	rBV2	40796	78791	17.61%	2.128%
11	7.317	1939	1952	1971	rBV	208702	373027	83.35%	10.077%
12	7.397	1972	1977	1989	rVB4	3486	6827	1.53%	0.184%
13	7.625	2039	2048	2063	rBV2	22779	42560	9.51%	1.150%
14	7.940	2131	2146	2153	rBV5	3866	7174	1.60%	0.194%
15	8.091	2183	2193	2226	rBV	134712	303531	67.82%	8.199%
16	8.850	2418	2429	2454	rBV	250086	413180	92.32%	11.161%
17	10.214	2841	2853	2865	rBV	64254	103495	23.13%	2.796%
18	10.378	2894	2904	2915	rBV3	7519	11858	2.65%	0.320%
19	11.249	3163	3175	3192	rBV	229947	355102	79.35%	9.592%
20	11.622	3279	3291	3309	rBV	195109	310100	69.29%	8.377%
21	12.345	3509	3516	3528	rVB6	4622	7267	1.62%	0.196%




Sum of corrected areas: 3701872

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025266.D
Acq On : 28 Mar 2022 17:08
Operator : SY/MD
Sample : N2101-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

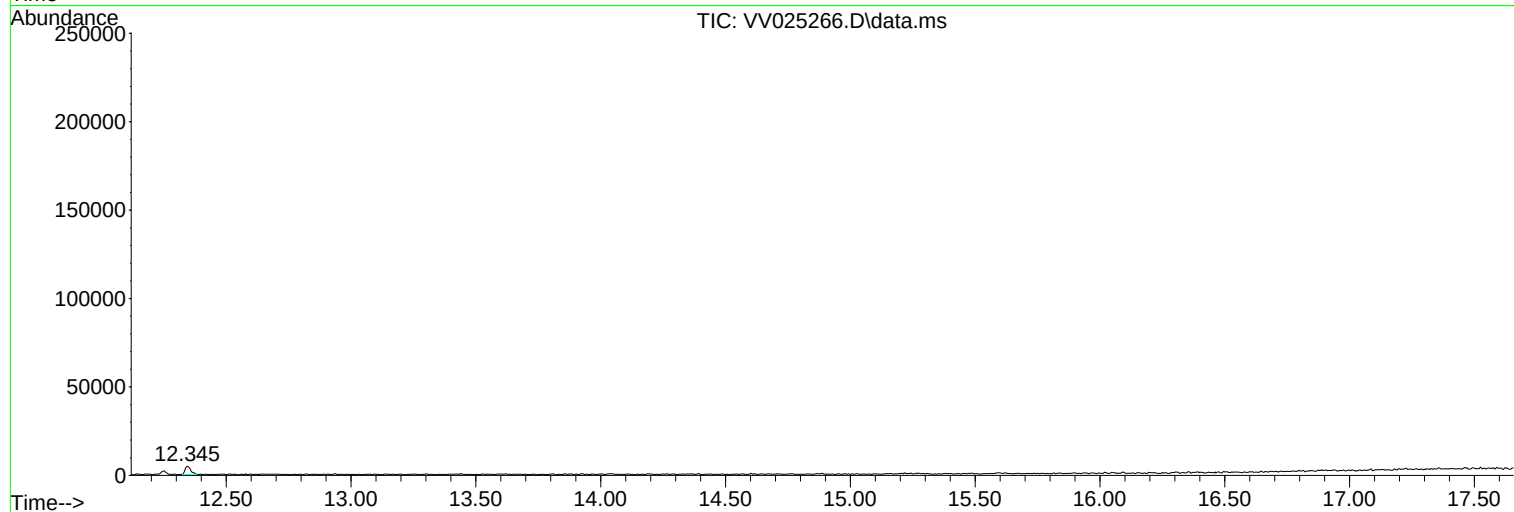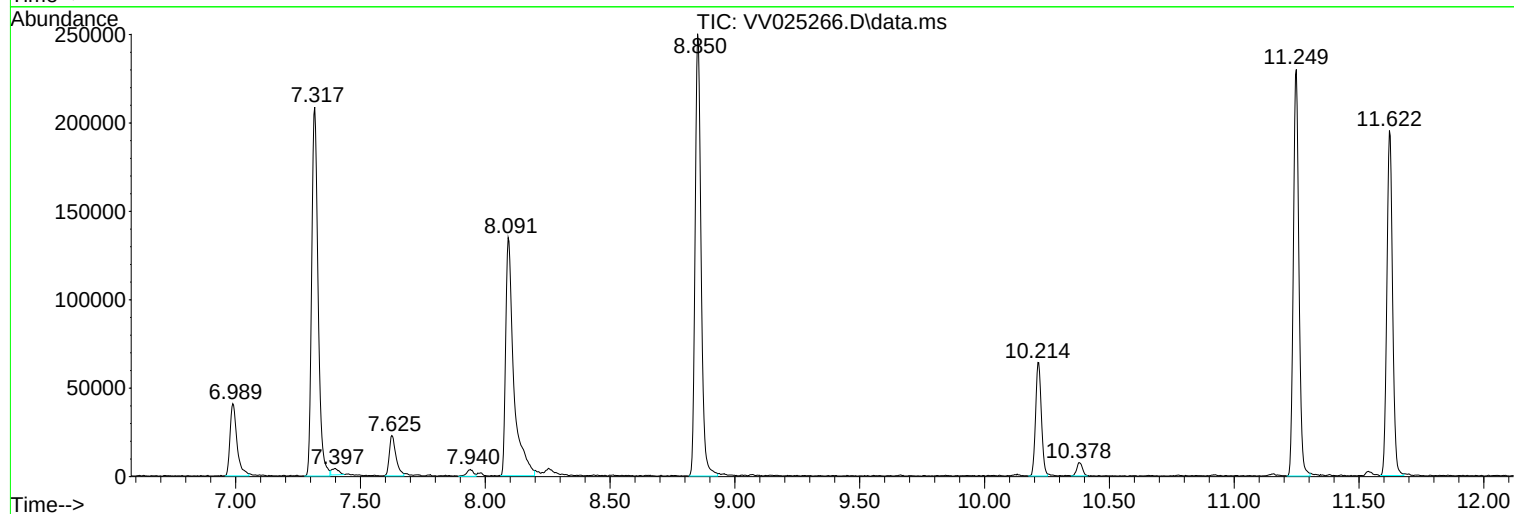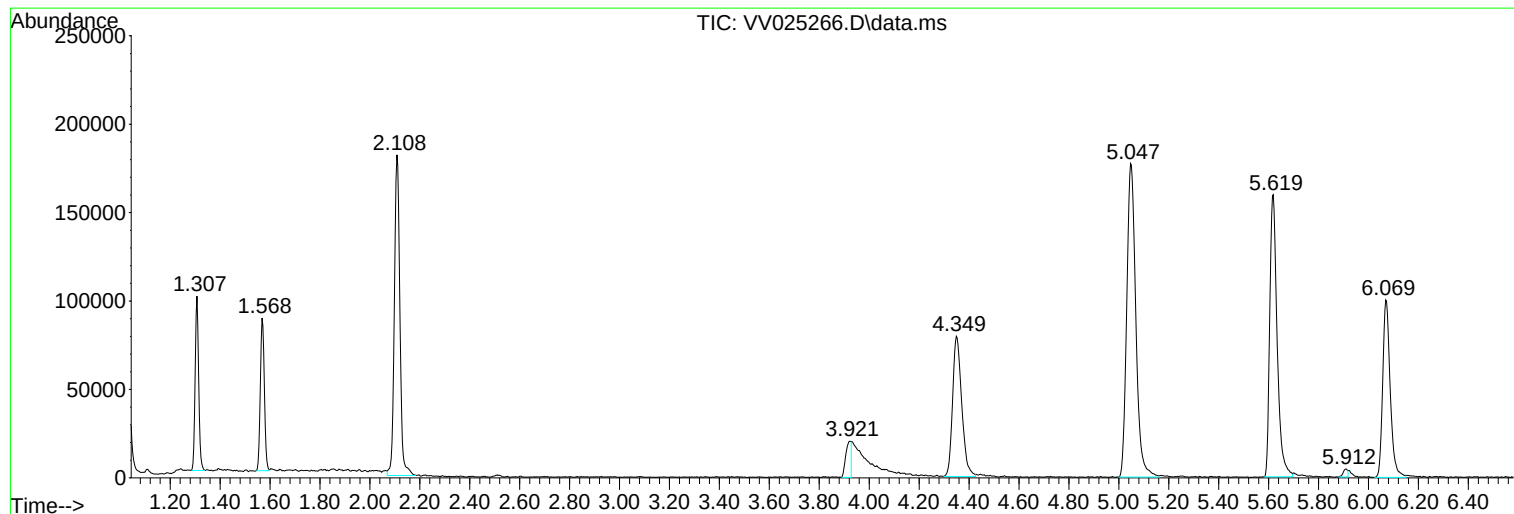

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025266.D
Acq On : 28 Mar 2022 17:08
Operator : SY/MD
Sample : N2101-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025266.D
Acq On : 28 Mar 2022 17:08
Operator : SY/MD
Sample : N2101-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
