

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025267.D
 Acq On : 28 Mar 2022 17:31
 Operator : SY/MD
 Sample : N2101-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAYW8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rBV	89234	90841	20.75%	2.427%
2	1.571	156	165	176	rBV	80301	90992	20.79%	2.431%
3	1.635	180	185	194	rVB5	3415	4869	1.11%	0.130%
4	2.111	323	333	354	rVB	170017	263000	60.08%	7.027%
5	3.153	646	657	675	rBV2	10671	26069	5.96%	0.697%
6	3.915	882	894	926	rBV2	24796	107758	24.62%	2.879%
7	4.352	1013	1030	1052	rBV	76727	195622	44.69%	5.227%
8	5.050	1231	1247	1280	rBV3	172995	437717	100.00%	11.696%
9	5.616	1412	1423	1448	rBV	157445	323869	73.99%	8.654%
10	6.069	1551	1564	1585	rBV	99409	207863	47.49%	5.554%
11	6.989	1838	1850	1868	rBV2	40206	75174	17.17%	2.009%
12	7.317	1941	1952	1973	rBV	207169	366644	83.76%	9.797%
13	7.625	2036	2048	2065	rBV3	22224	41394	9.46%	1.106%
14	8.092	2183	2193	2233	rBV	142483	311828	71.24%	8.332%
15	8.773	2394	2405	2415	rBV3	9159	14917	3.41%	0.399%
16	8.850	2415	2429	2454	rBV	249678	409724	93.60%	10.948%
17	10.214	2843	2853	2868	rBV	69664	110292	25.20%	2.947%
18	10.381	2896	2905	2914	rVB3	5198	7896	1.80%	0.211%
19	11.249	3164	3175	3193	rBV	220712	345447	78.92%	9.230%
20	11.535	3255	3264	3270	rBV6	3068	4803	1.10%	0.128%
21	11.622	3279	3291	3309	rBV	197519	305830	69.87%	8.172%




Sum of corrected areas: 3742549

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025267.D
Acq On : 28 Mar 2022 17:31
Operator : SY/MD
Sample : N2101-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

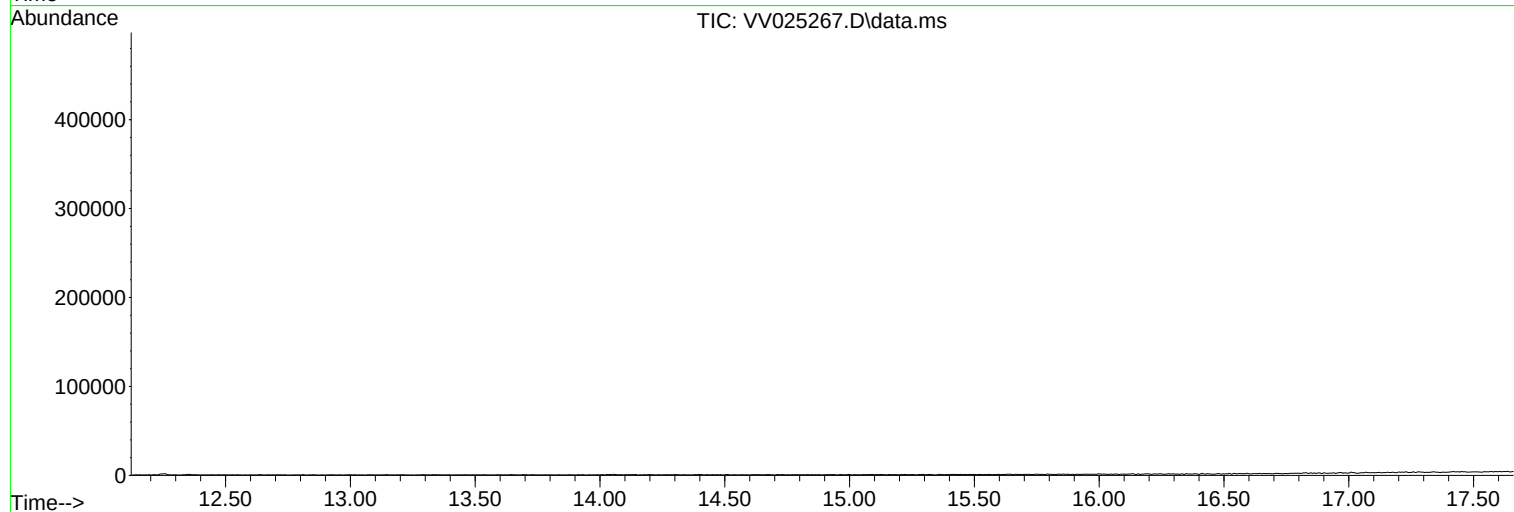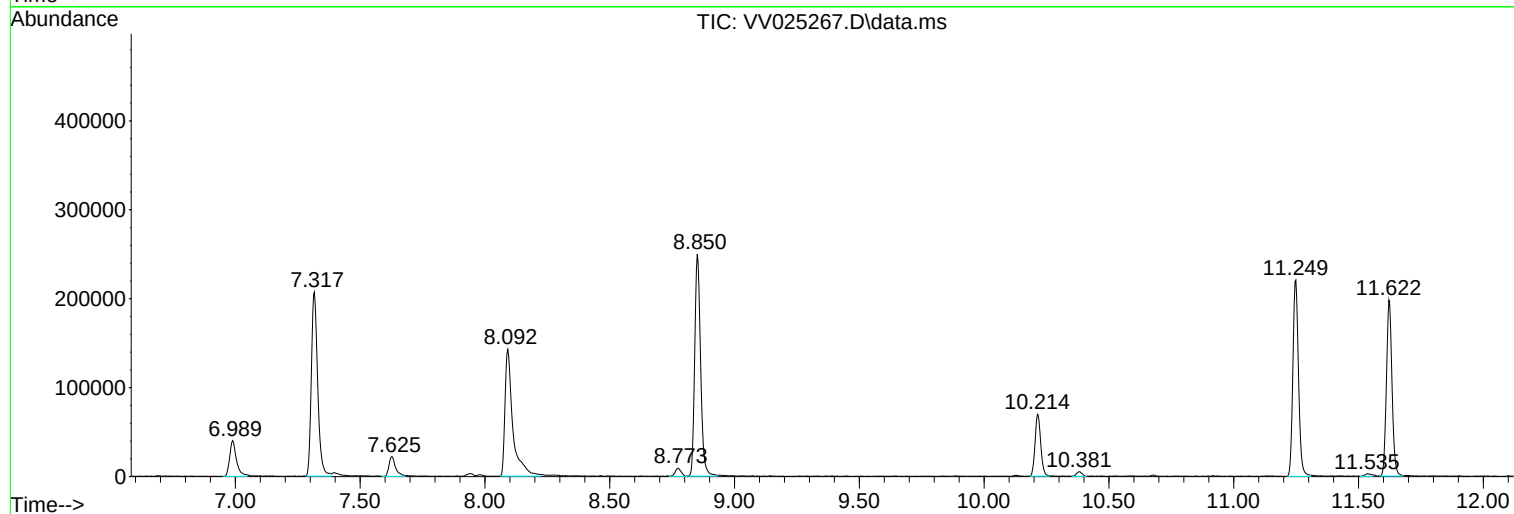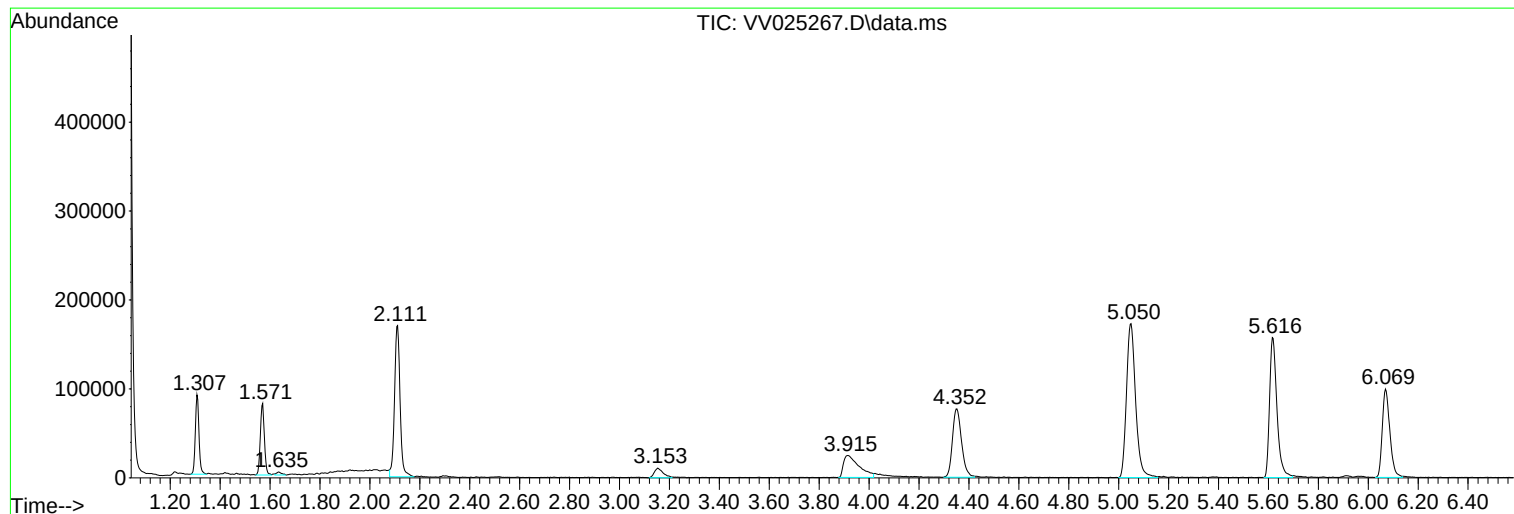

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025267.D
Acq On : 28 Mar 2022 17:31
Operator : SY/MD
Sample : N2101-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025267.D
Acq On : 28 Mar 2022 17:31
Operator : SY/MD
Sample : N2101-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc