

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025275.D
 Acq On : 28 Mar 2022 21:01
 Operator : SY/MD
 Sample : VV0328WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK328

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	94	rBV	91128	92304	19.94%	2.461%
2	1.571	156	165	178	rVB	82479	97257	21.01%	2.593%
3	2.111	322	333	350	rVB	171953	251638	54.36%	6.709%
4	2.510	450	457	466	rVB4	3474	5283	1.14%	0.141%
5	3.908	882	892	931	rBV2	28354	113837	24.59%	3.035%
6	4.352	1012	1030	1056	rBV2	82985	210207	45.41%	5.604%
7	5.047	1230	1246	1275	rBV3	183466	462889	100.00%	12.340%
8	5.619	1412	1424	1444	rBV2	153686	314167	67.87%	8.376%
9	5.912	1507	1515	1527	rVB7	3462	7165	1.55%	0.191%
10	6.069	1550	1564	1587	rBV	103207	217413	46.97%	5.796%
11	6.989	1839	1850	1870	rBV	41885	81236	17.55%	2.166%
12	7.317	1941	1952	1971	rBV	218825	389029	84.04%	10.371%
13	7.625	2038	2048	2064	rBV2	22453	43115	9.31%	1.149%
14	8.091	2183	2193	2225	rBV	147467	309686	66.90%	8.256%
15	8.850	2418	2429	2451	rBV	236086	392225	84.73%	10.457%
16	10.214	2842	2853	2867	rBV	68190	108519	23.44%	2.893%
17	11.246	3164	3174	3190	rBV	215101	337526	72.92%	8.998%
18	11.622	3278	3291	3309	rBV	200189	317506	68.59%	8.465%




Sum of corrected areas: 3751002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025275.D
Acq On : 28 Mar 2022 21:01
Operator : SY/MD
Sample : VV0328WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK328

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

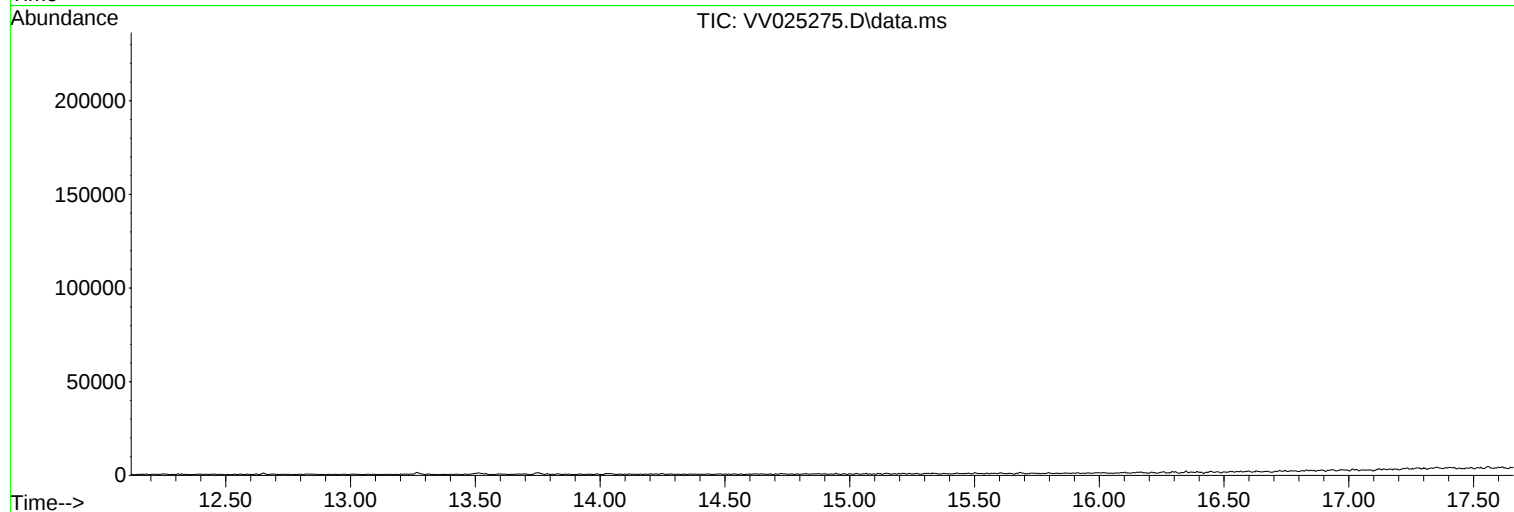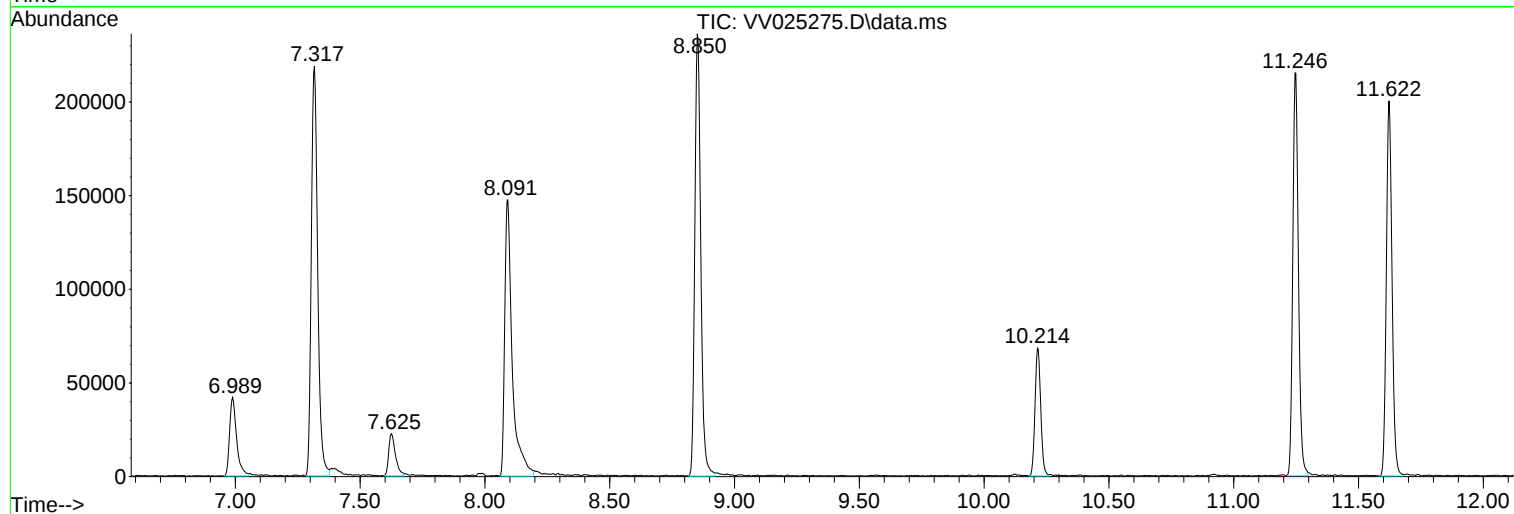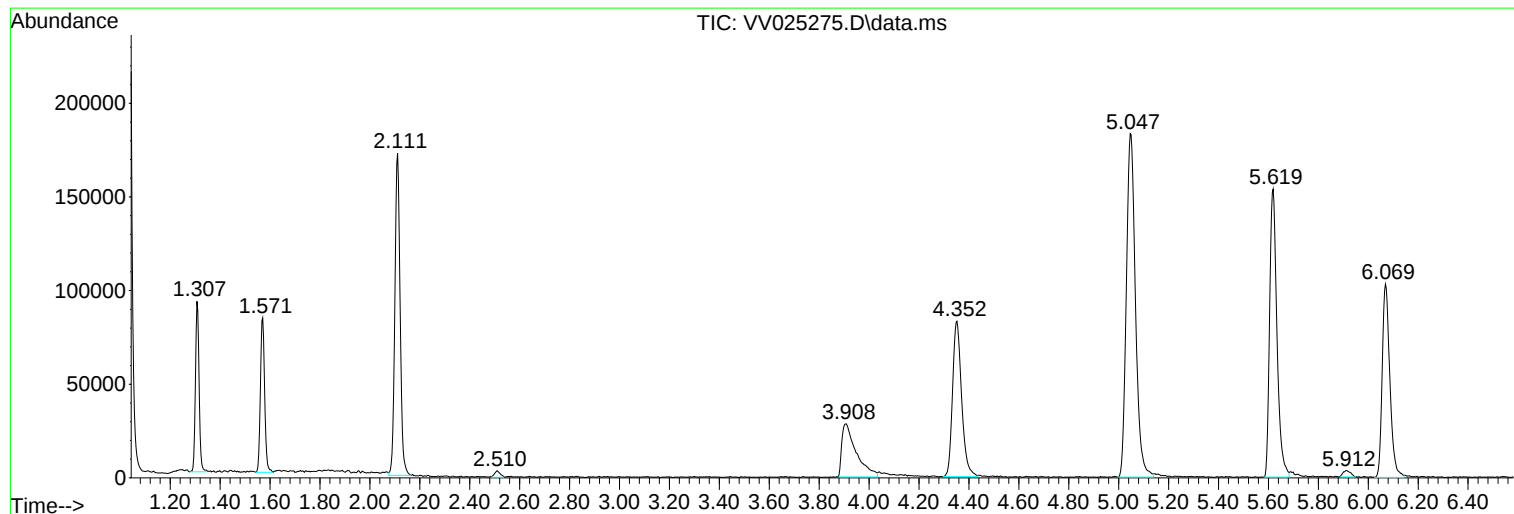

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025275.D
Acq On : 28 Mar 2022 21:01
Operator : SY/MD
Sample : VV0328WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK328

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
Data File : VV025275.D
Acq On : 28 Mar 2022 21:01
Operator : SY/MD
Sample : VV0328WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK328

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
