


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032822\
 Data File : VV025248.D
 Acq On : 28 Mar 2022 09:02
 Operator : SY/MD
 Sample : BFB289
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB289

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Apr 02 00:37:35 2022

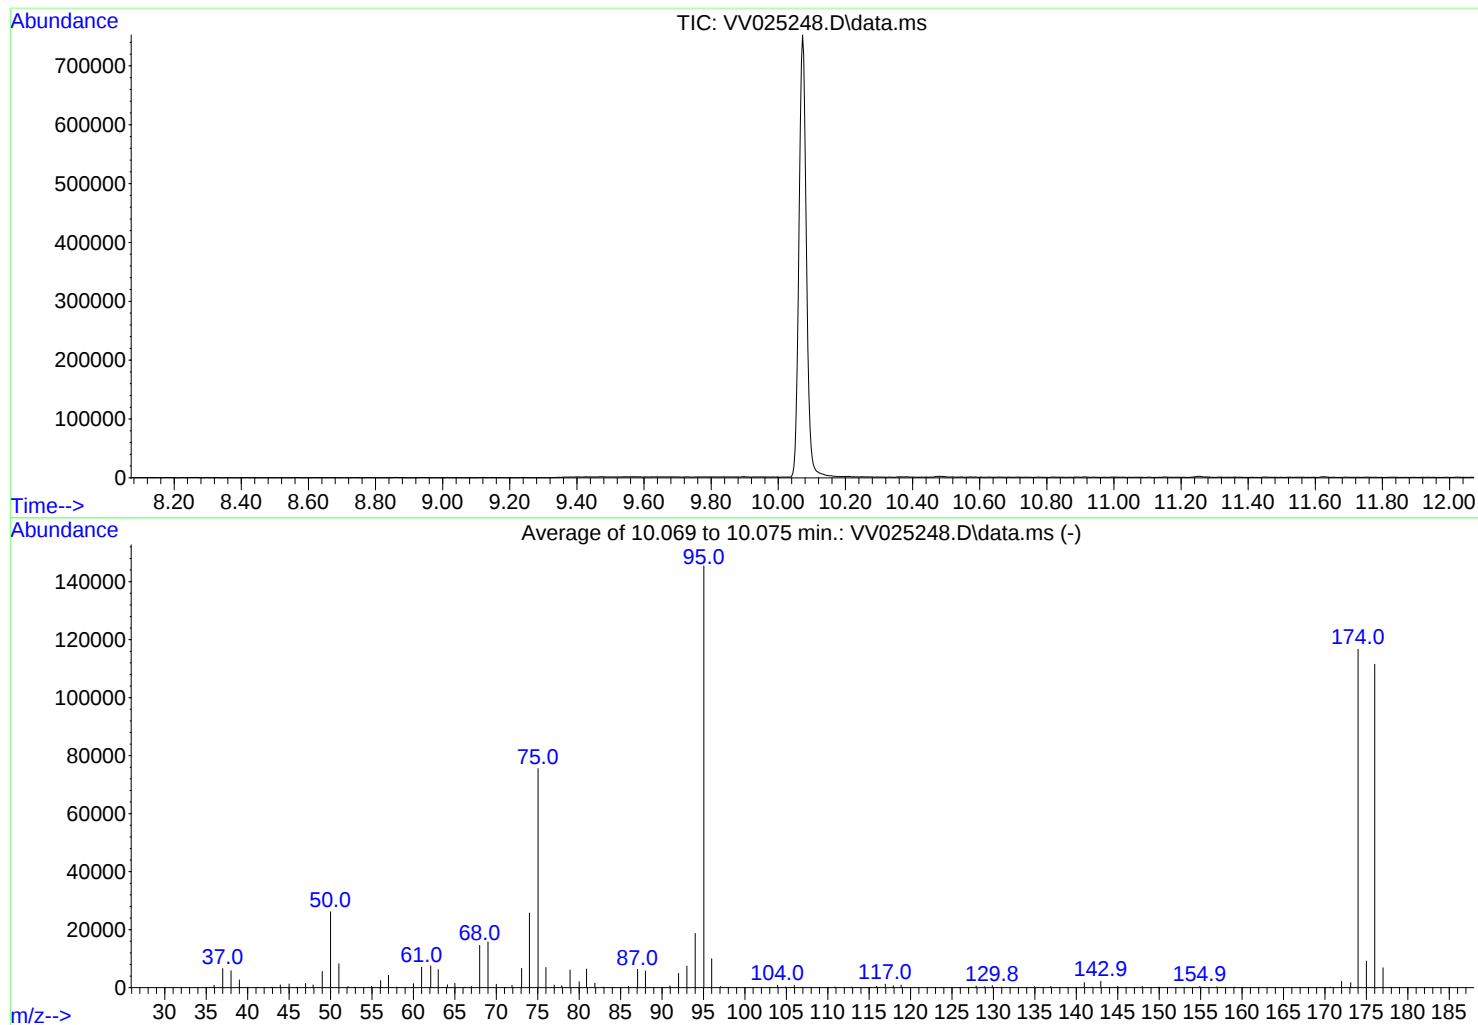

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	26155	PASS
75	95	30	80	51.9	75539	PASS
95	95	100	100	100.0	145451	PASS
96	95	5	9	6.8	9942	PASS
173	174	0.00	2	1.5	1704	PASS
174	95	50	120	80.2	116696	PASS
175	174	5	9	7.8	9157	PASS
176	174	95	105	95.5	111496	PASS
177	176	5	10	6.1	6822	PASS

m/z	Abundance
35.90	670.0
36.70	106.0
38.00	280.0
39.90	158.0
43.80	231.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.00	1515.0
37.00	6591.0
38.00	6318.0
39.00	2669.0
40.10	317.0
41.20	104.0
42.80	129.0
44.00	1125.0
45.00	1190.0
45.90	232.0
47.00	1509.0
47.90	984.0
49.00	5760.0
50.00	26128.0
51.00	8173.0
52.10	451.0
52.90	149.0
55.00	434.0
56.00	2363.0
57.00	4190.0
58.00	236.0
60.00	1419.0
61.00	6962.0
62.10	7470.0
63.00	6329.0
64.10	1115.0
65.00	1512.0
66.20	232.0
66.90	449.0
68.00	14254.0
69.00	15367.0
70.00	1228.0
71.10	150.0
71.90	799.0
73.00	6692.0
74.00	25400.0
75.10	74384.0
76.00	6681.0
77.00	835.0
77.90	635.0
78.90	6033.0
80.00	1964.0
80.90	6395.0
81.90	1579.0
82.90	249.0
85.90	339.0
87.10	6041.0
88.00	5428.0
90.90	580.0
92.00	4826.0
93.00	7211.0
94.00	18296.0
95.10	142144.0
96.00	9621.0
97.10	335.0
104.00	784.0
104.90	285.0
105.90	765.0
106.90	149.0
109.80	111.0
110.10	107.0
110.90	255.0
111.90	156.0
112.90	191.0
114.70	110.0
115.90	479.0
117.00	1146.0
117.90	624.0
118.80	865.0
123.80	131.0
127.90	661.0
129.00	349.0
129.80	628.0
130.90	239.0
135.00	354.0
135.80	121.0
136.90	408.0
138.80	116.0
140.00	125.0
140.90	1609.0
141.90	188.0
142.90	2142.0
144.10	184.0
145.00	456.0
146.10	230.0
147.00	183.0
148.00	440.0
149.00	134.0
150.00	201.0
152.00	130.0
153.00	215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.00	1549.0
37.00	6866.0
38.00	6357.0
39.00	2781.0
40.10	332.0
41.20	116.0
42.90	130.0
44.00	1199.0
45.00	1319.0
45.90	186.0
47.00	1492.0
47.90	1000.0
49.00	5737.0
50.00	27064.0
51.00	8530.0
52.10	429.0
52.90	164.0
54.90	449.0
56.00	2530.0
57.00	4335.0
58.00	229.0
60.00	1397.0
61.00	7188.0
62.10	7856.0
63.00	6430.0
64.10	1047.0
65.00	1555.0
66.20	206.0
67.00	382.0
68.00	15133.0
69.00	16488.0
70.00	1204.0
71.20	118.0
71.90	827.0
73.00	6757.0
74.00	26656.0
75.10	78200.0
76.00	7289.0
77.00	959.0
77.90	684.0
78.90	6270.0
80.00	2183.0
80.90	6616.0
81.90	1619.0
82.90	260.0
86.00	403.0
87.00	6517.0
88.00	5928.0
91.00	627.0
92.00	5138.0
93.00	7783.0
94.00	19360.0
95.10	150400.0
96.00	10417.0
97.00	368.0
103.90	855.0
104.90	307.0
106.00	829.0
106.90	169.0
110.10	136.0
110.90	283.0
111.90	132.0
112.90	266.0
115.10	146.0
115.90	525.0
116.90	1202.0
117.90	695.0
118.90	925.0
123.80	136.0
127.90	635.0
128.90	364.0
129.90	748.0
131.00	213.0
134.90	377.0
135.90	139.0
136.90	415.0
138.80	113.0
140.00	121.0
140.90	1888.0
141.90	204.0
142.90	2283.0
144.00	163.0
145.00	422.0
146.00	252.0
147.00	132.0
147.90	469.0
150.00	231.0
152.10	124.0
153.00	195.0
154.00	107.0
154.90	496.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

156.90	266.0
159.10	239.0
161.00	193.0
169.90	127.0
170.70	228.0
171.00	226.0
172.00	2264.0
173.10	1771.0
174.00	120880.0
175.00	9521.0
176.00	115672.0
177.00	7110.0
177.90	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.10	1527.0
37.00	6330.0
38.00	5709.0
39.00	2536.0
40.10	274.0
41.20	105.0
42.90	116.0
44.00	1135.0
45.00	1266.0
45.90	133.0
47.00	1336.0
47.90	818.0
49.00	5162.0
50.00	25272.0
51.00	7961.0
52.10	323.0
52.90	163.0
55.00	417.0
56.10	2369.0
57.00	4193.0
58.00	208.0
60.00	1317.0
61.00	6970.0
62.10	7226.0
63.00	5902.0
64.10	864.0
65.00	1436.0
66.20	136.0
67.10	349.0
68.00	14324.0
69.00	15526.0
70.00	1126.0
71.90	811.0
73.10	6380.0
74.00	25048.0
75.00	74032.0
76.00	6954.0
77.00	926.0
77.90	678.0
78.90	5889.0
80.00	2038.0
80.90	6228.0
81.90	1447.0
82.90	205.0
84.10	100.0
86.00	389.0
87.00	6263.0
88.00	5839.0
90.90	624.0
92.00	4848.0
93.00	7430.0
94.00	18456.0
95.00	143808.0
96.00	9787.0
97.00	374.0
103.90	867.0
104.90	309.0
106.00	791.0
106.90	162.0
110.10	120.0
110.80	274.0
112.00	105.0
112.90	260.0
115.00	147.0
115.90	567.0
116.90	1146.0
117.90	649.0
118.90	878.0
123.70	149.0
125.90	107.0
127.90	526.0
128.80	325.0
129.90	774.0
131.00	226.0
134.90	339.0
136.00	105.0
136.90	364.0
139.90	113.0
141.00	1884.0
141.90	210.0
143.00	2161.0
144.00	128.0
145.00	371.0
145.90	261.0
147.90	448.0
149.90	254.0
153.00	146.0
154.00	115.0
154.90	439.0
156.00	101.0
156.90	304.0
159.20	255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

161.10	203.0
170.00	116.0
170.60	219.0
171.10	201.0
172.00	2098.0
173.10	1572.0
174.00	118104.0
175.00	9077.0
176.00	112944.0
177.00	6651.0
178.00	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289