

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034891.D
 Acq On : 28 Mar 2024 17:10
 Operator : SY/MD
 Sample : P1822-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 29 00:26:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 29 00:23:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	362295	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	354646	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	164076	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	148404	42.415	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.820%		
7) Chloroethane-d5	1.532	69	132051	43.452	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.900%		
11) 1,1-Dichloroethene-d2	2.060	65	66633	43.445	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.880%		
21) 2-Butanone-d5	3.790	46	139677	67.311	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	67.310%		
24) Chloroform-d	4.249	84	230658	39.209	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.420%		
26) 1,2-Dichloroethane-d4	4.941	65	147742	39.557	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.120%		
32) Benzene-d6	4.960	84	478420	40.160	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.320%		
36) 1,2-Dichloropropane-d6	5.989	67	149528	39.528	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	79.060%		
41) Toluene-d8	7.243	98	424210	39.541	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.080%#		
43) trans-1,3-Dichloroprop...	7.555	79	63829	34.708	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.420%		
47) 2-Hexanone-d5	8.027	63	94098	65.792	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	65.790%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	195693	37.566	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	75.140%		
66) 1,2-Dichlorobenzene-d4	11.558	152	153238	41.597	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.200%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	2164	0.761	ug/L #	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034891.D
Acq On : 28 Mar 2024 17:10
Operator : SY/MD
Sample : P1822-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 29 00:26:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 00:23:40 2024
Response via : Initial Calibration

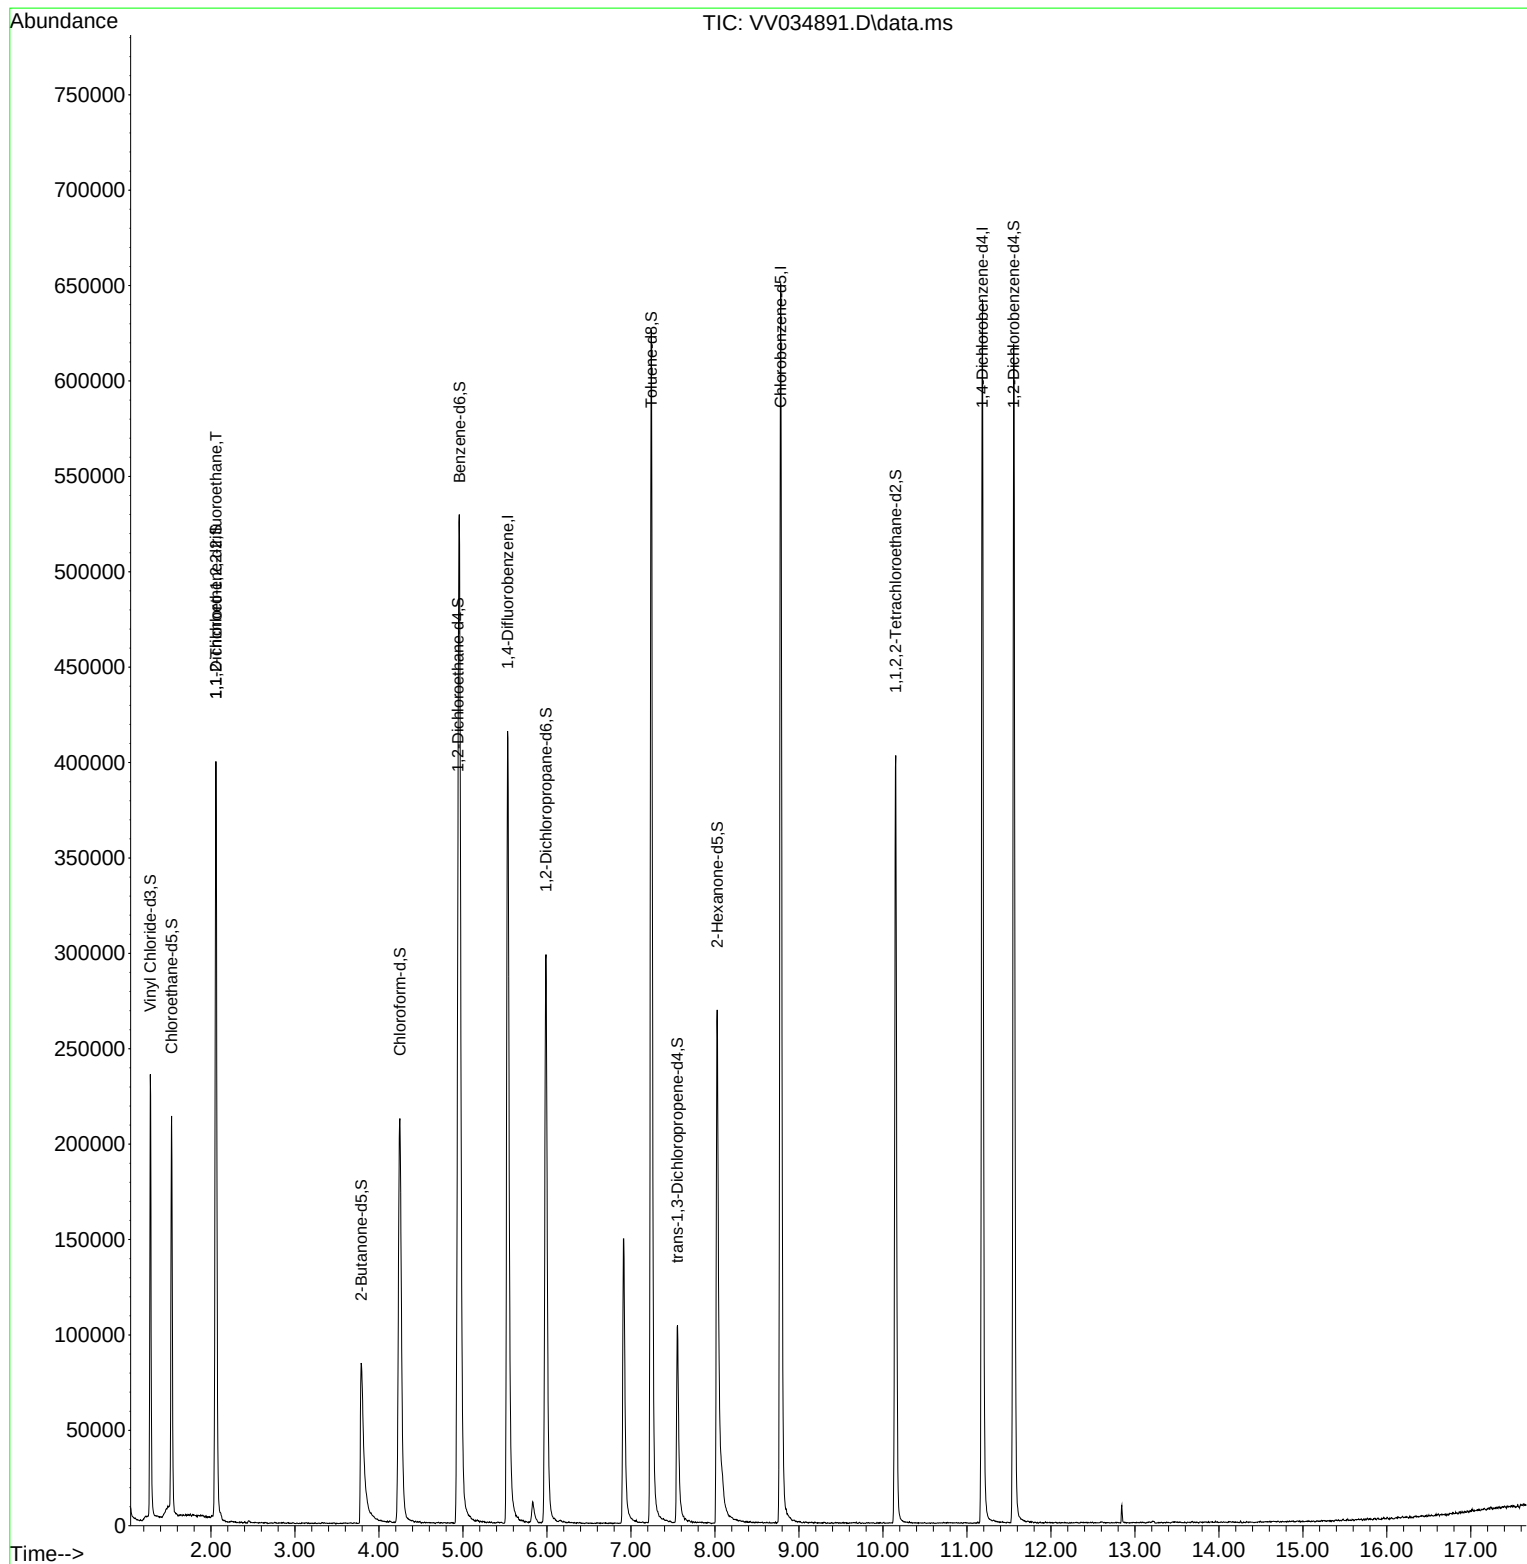

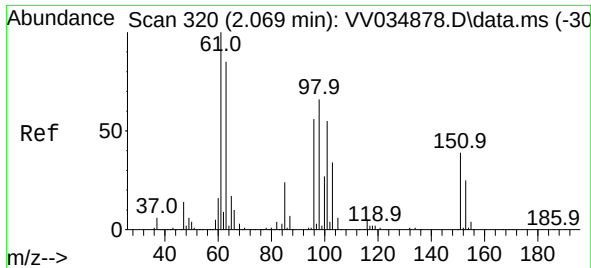

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.761 ug/L
 RT: 2.060 min Scan# 317
 Delta R.T. -0.010 min
 Lab File: VV034891.D
 Acq: 28 Mar 2024 17:10

Instrument :
 MSVOA_V
 ClientSampleId :

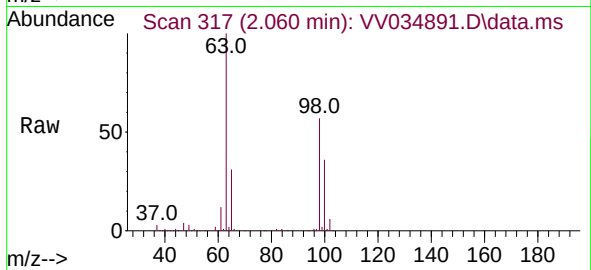

Tgt Ion:101 Resp: 2164
 Ion Ratio Lower Upper
 101 100
 85 0.0 35.3 52.9#
 151 0.0 55.0 82.4#

