

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034883.D
 Acq On : 28 Mar 2024 13:58
 Operator : SY/MD
 Sample : P1886-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	42	47	52	rBV	11562	10734	0.87%	0.108%
2	1.278	67	74	90	rVB	152559	167168	13.60%	1.678%
3	1.532	146	153	170	rVB	156632	183779	14.95%	1.845%
4	2.060	308	317	331	rBV	276724	395288	32.16%	3.967%
5	2.519	458	460	462	rBV	511	310	0.03%	0.003%
6	2.680	507	510	512	rBV2	303	192	0.02%	0.002%
7	2.780	538	541	546	rBV2	432	342	0.03%	0.003%
8	2.863	565	567	571	rVB2	378	336	0.03%	0.003%
9	2.902	571	579	580	rBV4	921	1021	0.08%	0.010%
10	2.953	591	595	596	rBV2	404	262	0.02%	0.003%
11	3.031	617	619	623	rBV4	213	149	0.01%	0.001%
12	3.101	636	641	642	rBV3	403	334	0.03%	0.003%
13	3.133	646	651	654	rVB3	511	479	0.04%	0.005%
14	3.153	654	657	658	rBV	314	168	0.01%	0.002%
15	3.162	658	660	664	rVB	352	193	0.02%	0.002%
16	3.185	664	667	672	rVB3	639	558	0.05%	0.006%
17	3.243	683	685	690	rBV2	377	256	0.02%	0.003%
18	3.278	695	696	699	rVB	530	271	0.02%	0.003%
19	3.297	699	702	704	rBV	339	139	0.01%	0.001%
20	3.346	713	717	718	rBV2	359	221	0.02%	0.002%
21	3.404	731	735	739	rBV3	379	357	0.03%	0.004%
22	3.461	751	753	762	rVB2	160	163	0.01%	0.002%
23	3.510	763	768	771	rVB2	418	347	0.03%	0.003%
24	3.532	772	775	778	rBV2	189	153	0.01%	0.002%
25	3.574	782	788	790	rBV3	569	483	0.04%	0.005%
26	3.732	833	837	839	rBV2	251	157	0.01%	0.002%
27	3.744	839	841	844	rBV2	447	303	0.02%	0.003%
28	3.786	846	854	886	rBV	102430	301755	24.55%	3.029%
29	4.249	982	998	1030	rBV2	212012	612211	49.81%	6.145%
30	4.616	1111	1112	1114	rBV	346	165	0.01%	0.002%
31	4.786	1163	1165	1170	rVB2	466	316	0.03%	0.003%
32	4.902	1199	1201	1202	rBV	338	170	0.01%	0.002%
33	4.953	1202	1217	1249	rVV2	458273	1229180	100.00%	12.337%
34	5.416	1358	1361	1366	rVB3	635	491	0.04%	0.005%
35	5.439	1366	1368	1370	rBV2	459	208	0.02%	0.002%
36	5.484	1379	1382	1385	rBV4	569	390	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034883.D
 Acq On : 28 Mar 2024 13:58
 Operator : SY/MD
 Sample : P1886-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1430	rBV	380076	796626	64.81%	7.996%
38	5.831	1481	1490	1506	rVB3	12228	27612	2.25%	0.277%
39	5.989	1526	1539	1567	rBV	280383	590390	48.03%	5.926%
40	6.201	1603	1605	1607	rBV	428	196	0.02%	0.002%
41	6.275	1625	1628	1629	rBV2	421	180	0.01%	0.002%
42	6.310	1638	1639	1640	rBV2	437	158	0.01%	0.002%
43	6.445	1671	1681	1696	rBV4	7345	16211	1.32%	0.163%
44	6.558	1714	1716	1721	rVB2	320	222	0.02%	0.002%
45	6.635	1736	1740	1742	rBV3	499	432	0.04%	0.004%
46	6.677	1749	1753	1755	rBV2	537	283	0.02%	0.003%
47	6.690	1755	1757	1761	rVB	498	190	0.02%	0.002%
48	6.709	1761	1763	1766	rVB2	549	270	0.02%	0.003%
49	6.728	1767	1769	1771	rBV	219	122	0.01%	0.001%
50	6.796	1787	1790	1792	rBV3	347	258	0.02%	0.003%
51	6.860	1807	1810	1816	rBV2	388	413	0.03%	0.004%
52	6.911	1816	1826	1858	rBV	136877	272584	22.18%	2.736%
53	7.194	1913	1914	1918	rBV2	628	467	0.04%	0.005%
54	7.243	1918	1929	1951	rBV	508068	898594	73.11%	9.019%
55	7.555	2017	2026	2050	rBV	95394	180541	14.69%	1.812%
56	7.751	2084	2087	2090	rBV4	538	449	0.04%	0.005%
57	7.841	2111	2115	2117	rBV3	434	283	0.02%	0.003%
58	7.879	2119	2127	2136	rVB3	2492	4294	0.35%	0.043%
59	7.931	2141	2143	2144	rBV3	392	183	0.01%	0.002%
60	7.947	2146	2148	2152	rVB2	646	412	0.03%	0.004%
61	7.973	2152	2156	2158	rBV	166	133	0.01%	0.001%
62	7.992	2158	2162	2163	rBV2	509	351	0.03%	0.004%
63	8.024	2163	2172	2213	rBV2	311898	678171	55.17%	6.807%
64	8.554	2335	2337	2338	rBV2	521	271	0.02%	0.003%
65	8.606	2351	2353	2358	rVB2	723	410	0.03%	0.004%
66	8.635	2358	2362	2365	rBV3	456	341	0.03%	0.003%
67	8.648	2365	2366	2367	rBV3	386	116	0.01%	0.001%
68	8.686	2376	2378	2380	rBV2	501	226	0.02%	0.002%
69	8.783	2396	2408	2438	rBV	602118	1006182	81.86%	10.099%
70	9.136	2516	2518	2519	rBV2	420	127	0.01%	0.001%
71	9.175	2527	2530	2532	rBV3	490	278	0.02%	0.003%
72	9.223	2543	2545	2549	rBV2	280	196	0.02%	0.002%
73	9.738	2702	2705	2708	rBV	256	192	0.02%	0.002%
74	9.757	2708	2711	2714	rVV	580	339	0.03%	0.003%
75	9.776	2714	2717	2719	rVV	239	149	0.01%	0.001%
76	9.808	2723	2727	2729	rBV	190	134	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034883.D
 Acq On : 28 Mar 2024 13:58
 Operator : SY/MD
 Sample : P1886-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.934	2763	2766	2769	rBV3	395	254	0.02%	0.003%
78	10.098	2815	2817	2821	rVB2	387	269	0.02%	0.003%
79	10.152	2821	2834	2858	rBV	439482	703268	57.21%	7.059%
80	10.326	2879	2888	2900	rVB2	4091	6494	0.53%	0.065%
81	10.416	2914	2916	2919	rBV	396	222	0.02%	0.002%
82	10.455	2926	2928	2929	rBV	325	124	0.01%	0.001%
83	10.477	2933	2935	2938	rBV3	911	518	0.04%	0.005%
84	10.644	2984	2987	2989	rBV2	529	305	0.02%	0.003%
85	10.776	3026	3028	3031	rVB2	309	133	0.01%	0.001%
86	11.133	3131	3139	3142	rBV5	1357	1925	0.16%	0.019%
87	11.185	3144	3155	3184	rVV	608693	945408	76.91%	9.489%
88	11.461	3238	3241	3245	rBV3	472	516	0.04%	0.005%
89	11.558	3259	3271	3297	rBV	564866	905451	73.66%	9.088%
90	11.988	3400	3405	3408	rBV2	541	604	0.05%	0.006%
91	12.050	3422	3424	3428	rBV2	315	168	0.01%	0.002%
92	12.188	3463	3467	3468	rBV2	455	376	0.03%	0.004%
93	12.320	3504	3508	3511	rBV2	791	750	0.06%	0.008%
94	12.474	3554	3556	3561	rBV2	405	332	0.03%	0.003%
95	12.525	3567	3572	3573	rBV	490	396	0.03%	0.004%
96	12.567	3582	3585	3587	rVB3	377	185	0.02%	0.002%
97	12.593	3587	3593	3600	rBV6	1656	2228	0.18%	0.022%
98	12.734	3634	3637	3639	rBV2	551	281	0.02%	0.003%
99	13.451	3856	3860	3870	rVB3	3475	4570	0.37%	0.046%
100	13.905	3998	4001	4004	rBV	845	516	0.04%	0.005%




Sum of corrected areas: 9963328

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034883.D
Acq On : 28 Mar 2024 13:58
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

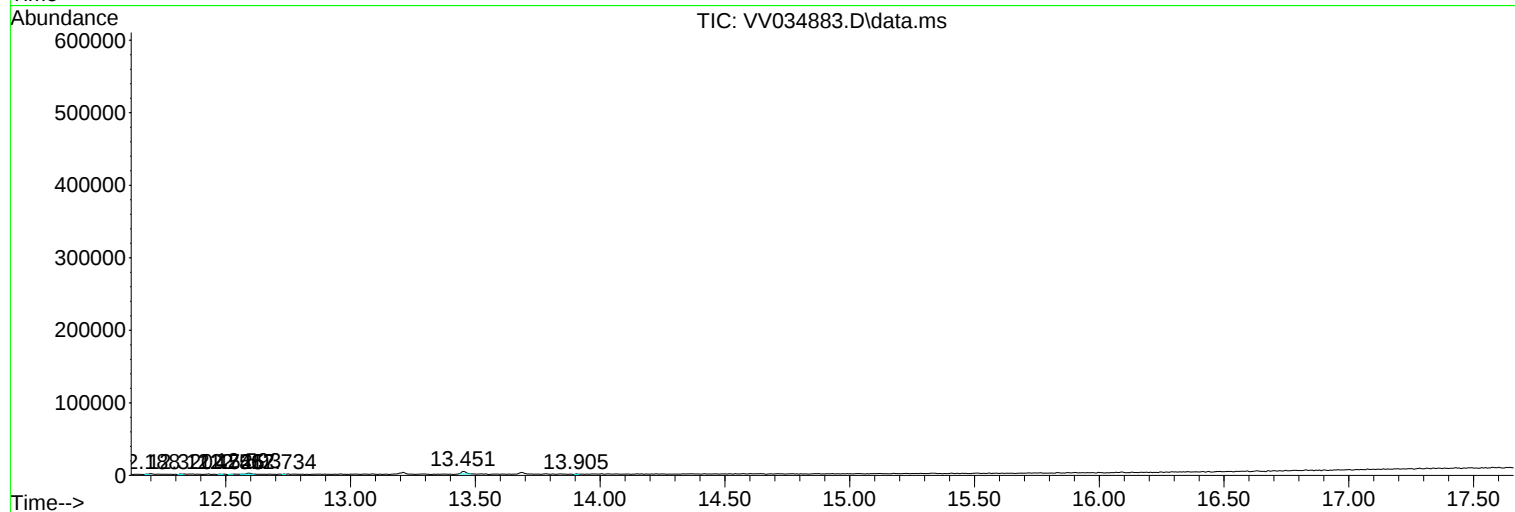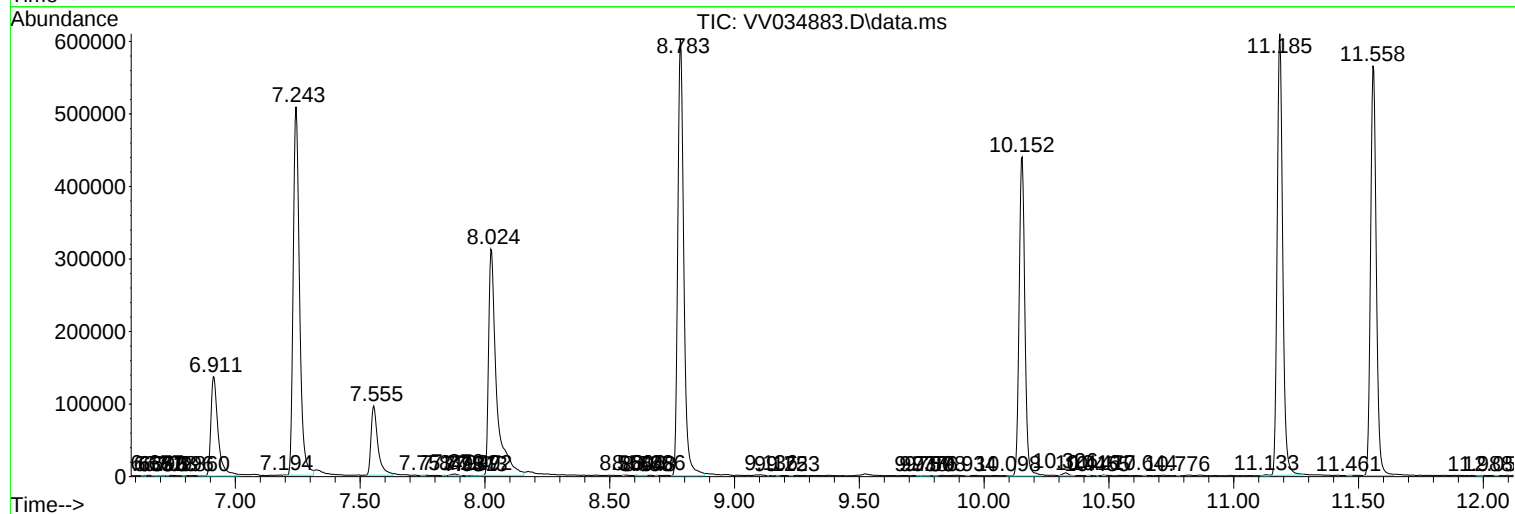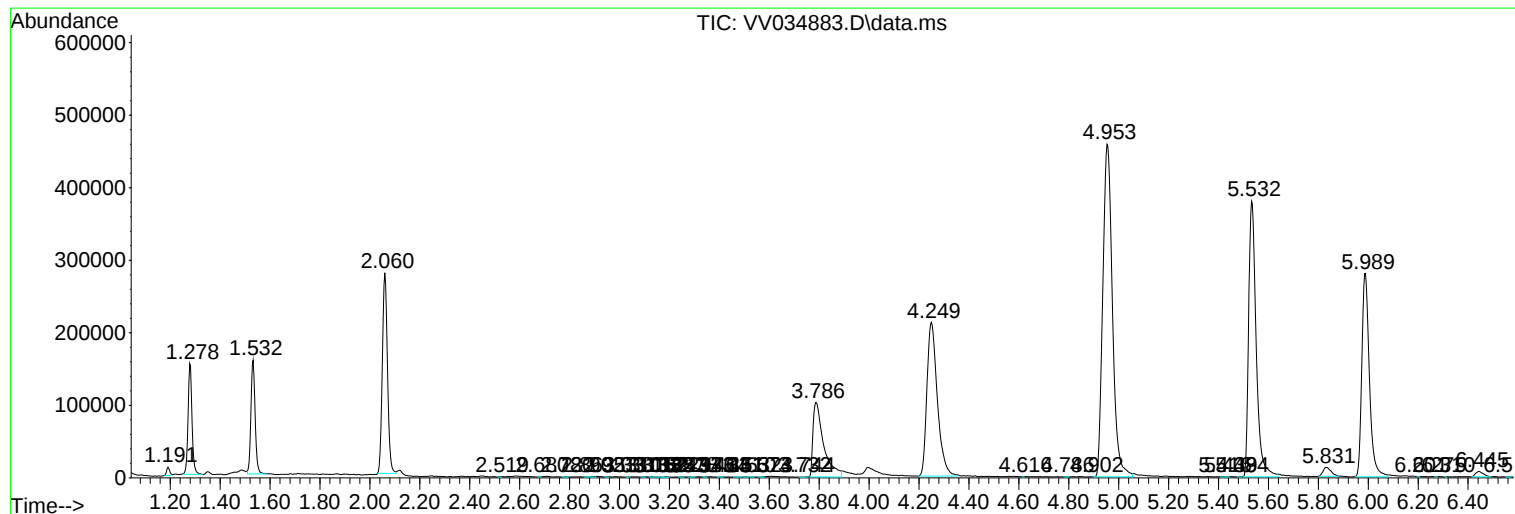

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034883.D
Acq On : 28 Mar 2024 13:58
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034883.D
Acq On : 28 Mar 2024 13:58
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
