

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034884.D
 Acq On : 28 Mar 2024 14:22
 Operator : SY/MD
 Sample : P1886-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	42	47	53	rBV	11907	11933	0.97%	0.121%
2	1.278	66	74	89	rVB	151335	165271	13.39%	1.673%
3	1.532	146	153	173	rVB	159444	189586	15.36%	1.920%
4	2.059	308	317	331	rBV	269639	387844	31.43%	3.927%
5	2.336	399	403	404	rBV2	686	430	0.03%	0.004%
6	2.442	434	436	437	rBV	825	389	0.03%	0.004%
7	2.680	507	510	511	rBV	289	143	0.01%	0.001%
8	2.735	525	527	530	rBV2	328	262	0.02%	0.003%
9	2.809	547	550	551	rBV2	294	142	0.01%	0.001%
10	2.860	561	566	568	rBV4	492	406	0.03%	0.004%
11	2.876	568	571	573	rBV3	447	338	0.03%	0.003%
12	2.931	586	588	589	rBV2	362	154	0.01%	0.002%
13	3.014	612	614	615	rBV2	279	135	0.01%	0.001%
14	3.043	621	623	627	rBV2	411	345	0.03%	0.003%
15	3.063	627	629	632	rVB2	386	207	0.02%	0.002%
16	3.111	640	644	649	rBV2	558	487	0.04%	0.005%
17	3.162	658	660	661	rBV	386	119	0.01%	0.001%
18	3.172	661	663	669	rVB2	636	603	0.05%	0.006%
19	3.198	669	671	675	rBV3	351	279	0.02%	0.003%
20	3.217	675	677	679	rVV	238	119	0.01%	0.001%
21	3.249	683	687	688	rVV	196	162	0.01%	0.002%
22	3.259	688	690	692	rVV	302	148	0.01%	0.001%
23	3.272	692	694	697	rVB	328	145	0.01%	0.001%
24	3.310	703	706	709	rBV	369	230	0.02%	0.002%
25	3.323	709	710	711	rBV	399	122	0.01%	0.001%
26	3.346	714	717	722	rVB3	422	342	0.03%	0.003%
27	3.394	729	732	736	rVV2	344	232	0.02%	0.002%
28	3.458	748	752	755	rBV2	452	363	0.03%	0.004%
29	3.487	759	761	765	rVV	229	145	0.01%	0.001%
30	3.693	822	825	827	rVB	248	131	0.01%	0.001%
31	3.789	845	855	899	rBV	98777	303990	24.64%	3.078%
32	4.249	981	998	1035	rBV3	210280	611772	49.58%	6.194%
33	4.545	1085	1090	1093	rBV	930	862	0.07%	0.009%
34	4.651	1120	1123	1124	rBV2	360	192	0.02%	0.002%
35	4.677	1127	1131	1132	rBV3	281	158	0.01%	0.002%
36	4.735	1147	1149	1153	rVB2	498	231	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034884.D
 Acq On : 28 Mar 2024 14:22
 Operator : SY/MD
 Sample : P1886-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.780	1160	1163	1165	rBV2	206	120	0.01%	0.001%
38	4.809	1165	1172	1173	rBV3	458	454	0.04%	0.005%
39	4.863	1183	1189	1192	rBV3	523	579	0.05%	0.006%
40	4.956	1201	1218	1260	rBV2	457484	1233918	100.00%	12.494%
41	5.365	1343	1345	1348	rBV3	312	151	0.01%	0.002%
42	5.445	1368	1370	1373	rBV2	347	203	0.02%	0.002%
43	5.532	1386	1397	1430	rBV	381910	797040	64.59%	8.070%
44	5.834	1480	1491	1514	rVB2	14193	32897	2.67%	0.333%
45	5.989	1525	1539	1566	rBV	280092	583020	47.25%	5.903%
46	6.288	1626	1632	1634	rBV4	674	627	0.05%	0.006%
47	6.307	1635	1638	1640	rBV	424	275	0.02%	0.003%
48	6.355	1649	1653	1654	rBV2	487	252	0.02%	0.003%
49	6.445	1670	1681	1694	rBV2	7589	16123	1.31%	0.163%
50	6.532	1706	1708	1712	rVB	417	208	0.02%	0.002%
51	6.603	1727	1730	1731	rVB2	244	125	0.01%	0.001%
52	6.625	1731	1737	1741	rBV4	746	861	0.07%	0.009%
53	6.686	1754	1756	1759	rBV2	367	197	0.02%	0.002%
54	6.722	1764	1767	1773	rVB4	497	562	0.05%	0.006%
55	6.751	1773	1776	1777	rBV	405	215	0.02%	0.002%
56	6.915	1814	1827	1851	rBV	137164	266384	21.59%	2.697%
57	7.243	1917	1929	1951	rBV	497361	886430	71.84%	8.975%
58	7.554	2017	2026	2049	rBV2	94747	178985	14.51%	1.812%
59	7.824	2107	2110	2111	rBV	428	232	0.02%	0.002%
60	7.853	2116	2119	2120	rBV2	720	408	0.03%	0.004%
61	7.940	2144	2146	2150	rVB3	447	208	0.02%	0.002%
62	7.969	2150	2155	2157	rBV2	599	463	0.04%	0.005%
63	8.027	2163	2173	2213	rBV2	296866	652261	52.86%	6.604%
64	8.686	2375	2378	2381	rVB3	702	451	0.04%	0.005%
65	8.783	2397	2408	2437	rBV	599685	996482	80.76%	10.089%
66	9.123	2512	2514	2517	rBV2	547	269	0.02%	0.003%
67	9.194	2534	2536	2539	rVB2	273	140	0.01%	0.001%
68	9.210	2539	2541	2542	rBV	401	196	0.02%	0.002%
69	9.259	2552	2556	2558	rBV2	601	359	0.03%	0.004%
70	9.287	2562	2565	2567	rBV2	441	237	0.02%	0.002%
71	9.458	2615	2618	2619	rBV	378	226	0.02%	0.002%
72	9.696	2690	2692	2693	rBV	340	115	0.01%	0.001%
73	9.770	2707	2715	2718	rBV2	456	511	0.04%	0.005%
74	9.815	2725	2729	2730	rBV2	418	275	0.02%	0.003%
75	9.976	2777	2779	2781	rBV2	349	210	0.02%	0.002%
76	10.082	2807	2812	2816	rBV3	441	355	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034884.D
 Acq On : 28 Mar 2024 14:22
 Operator : SY/MD
 Sample : P1886-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.152	2822	2834	2855	rBV	433201	686494	55.64%	6.951%
78	10.329	2881	2889	2897	rVB4	3528	5340	0.43%	0.054%
79	10.609	2974	2976	2981	rVB2	368	235	0.02%	0.002%
80	10.709	3004	3007	3010	rBV4	650	500	0.04%	0.005%
81	10.943	3075	3080	3083	rBV4	588	619	0.05%	0.006%
82	11.062	3114	3117	3121	rBV	529	427	0.03%	0.004%
83	11.082	3121	3123	3125	rBV2	312	159	0.01%	0.002%
84	11.133	3133	3139	3144	rBV5	1030	1493	0.12%	0.015%
85	11.184	3144	3155	3179	rBV	595796	937625	75.99%	9.494%
86	11.455	3234	3239	3244	rBV3	700	797	0.06%	0.008%
87	11.509	3252	3256	3259	rBV3	449	421	0.03%	0.004%
88	11.561	3260	3272	3296	rVV	565881	899537	72.90%	9.108%
89	11.828	3349	3355	3356	rBV4	499	463	0.04%	0.005%
90	12.017	3412	3414	3416	rBV2	465	247	0.02%	0.003%
91	12.345	3512	3516	3521	rBV4	704	842	0.07%	0.009%
92	12.422	3538	3540	3542	rBV	445	205	0.02%	0.002%
93	12.490	3558	3561	3565	rVB3	510	397	0.03%	0.004%
94	12.509	3565	3567	3569	rBV	292	131	0.01%	0.001%
95	12.548	3576	3579	3582	rBV	602	348	0.03%	0.004%
96	12.680	3617	3620	3622	rBV2	519	281	0.02%	0.003%
97	12.821	3662	3664	3668	rVB2	457	219	0.02%	0.002%
98	12.905	3688	3690	3693	rBV2	367	146	0.01%	0.001%
99	13.210	3778	3785	3794	rVB6	2749	3620	0.29%	0.037%
100	13.454	3854	3861	3870	rBV2	2833	4480	0.36%	0.045%




Sum of corrected areas: 9876467

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034884.D
Acq On : 28 Mar 2024 14:22
Operator : SY/MD
Sample : P1886-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

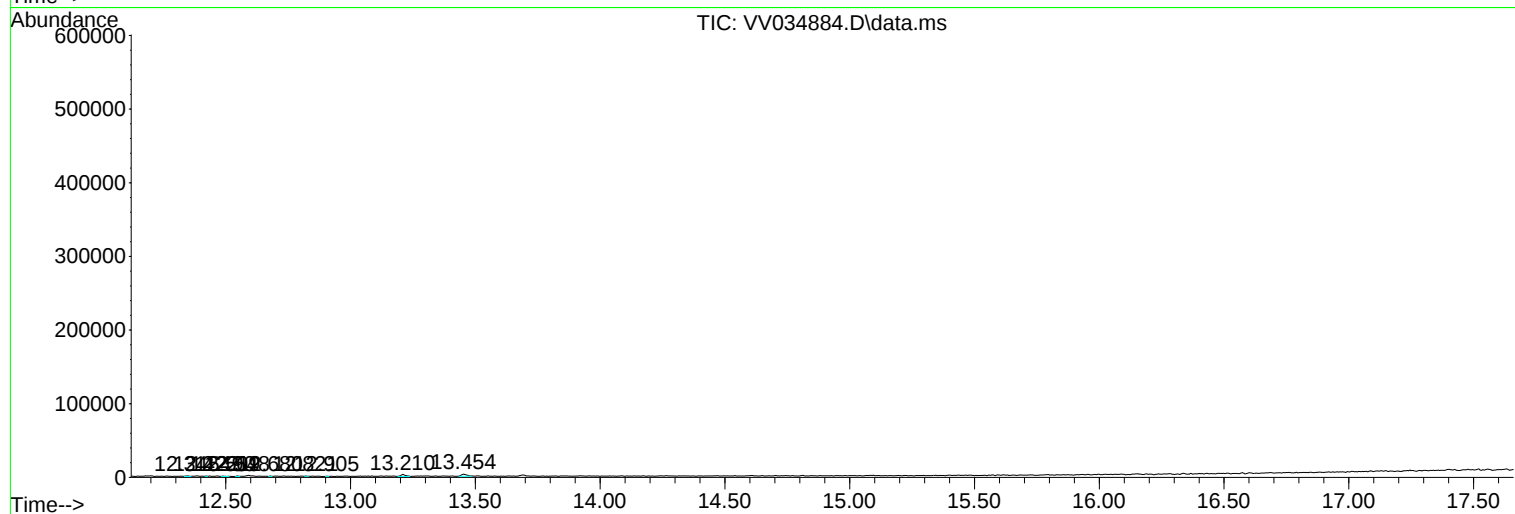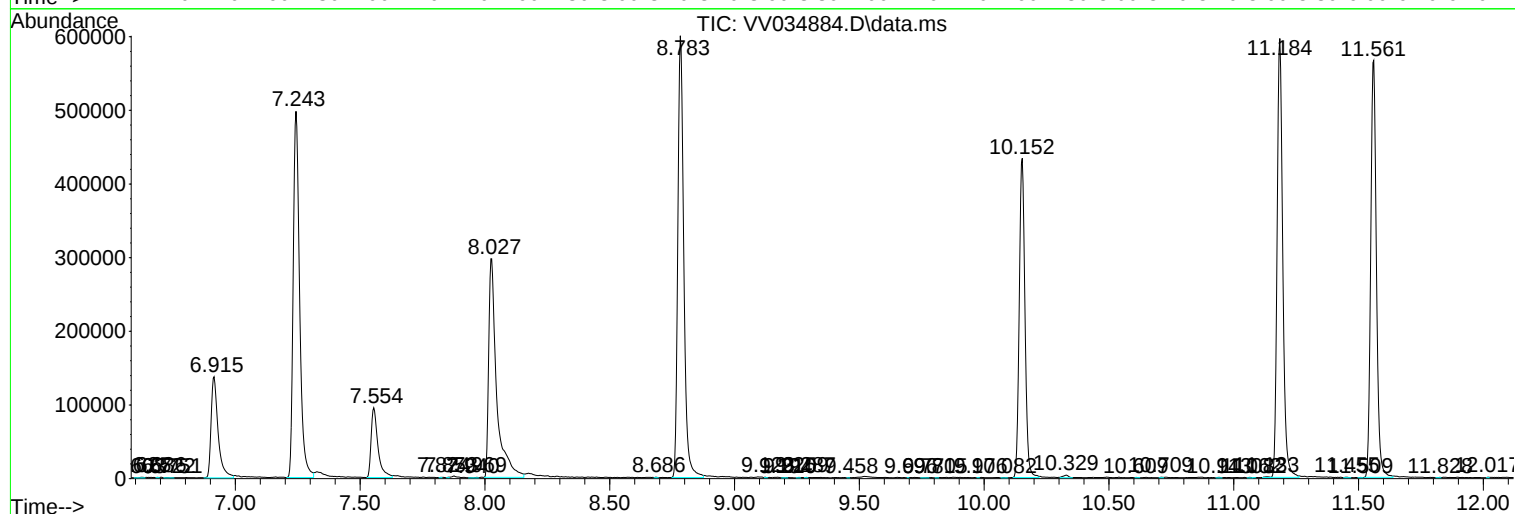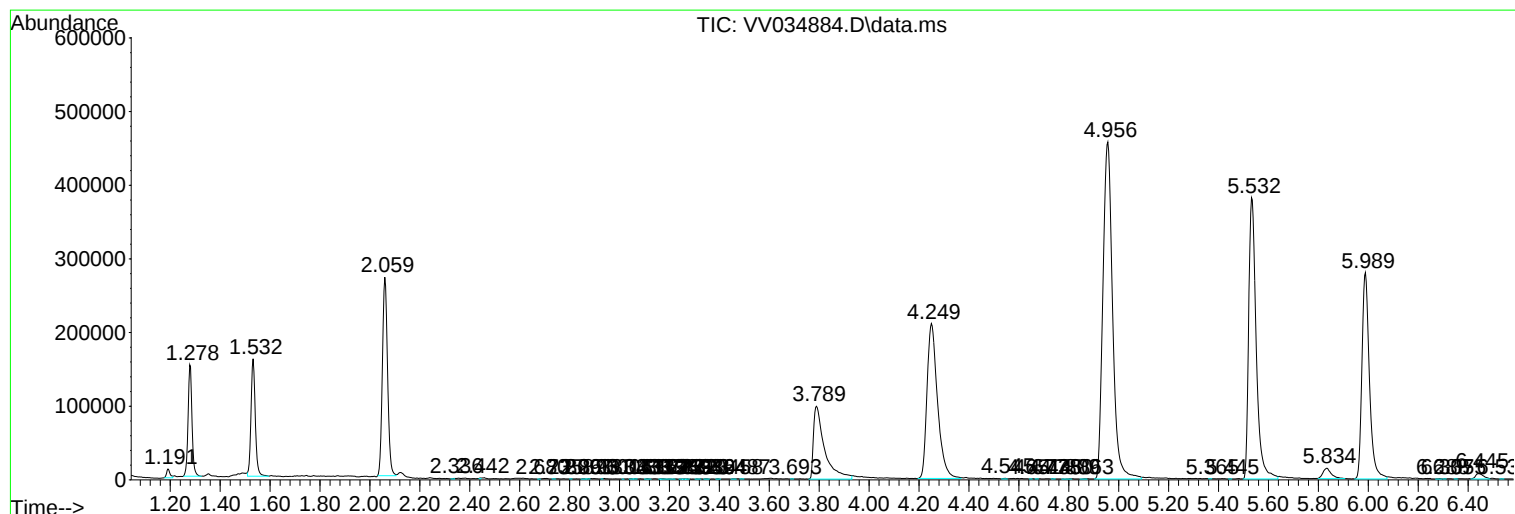

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034884.D
Acq On : 28 Mar 2024 14:22
Operator : SY/MD
Sample : P1886-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034884.D
Acq On : 28 Mar 2024 14:22
Operator : SY/MD
Sample : P1886-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc