

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034885.D
 Acq On : 28 Mar 2024 14:46
 Operator : SY/MD
 Sample : P1851-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	251859	266749	17.72%	2.382%
2	1.532	146	153	166	rVB	209080	243712	16.19%	2.176%
3	2.060	307	317	332	rBV	421371	611356	40.62%	5.459%
4	2.503	452	455	458	rBV2	677	563	0.04%	0.005%
5	2.606	484	487	490	rVB2	644	339	0.02%	0.003%
6	2.632	490	495	497	rBV2	428	357	0.02%	0.003%
7	2.687	508	512	513	rBV2	527	376	0.02%	0.003%
8	2.809	547	550	553	rBV3	403	321	0.02%	0.003%
9	2.879	569	572	577	rBV3	289	218	0.01%	0.002%
10	2.966	595	599	601	rBV2	379	307	0.02%	0.003%
11	3.014	611	614	617	rVB3	661	359	0.02%	0.003%
12	3.092	634	638	644	rVB2	436	483	0.03%	0.004%
13	3.198	666	671	673	rBV2	282	354	0.02%	0.003%
14	3.259	687	690	694	rVB2	338	240	0.02%	0.002%
15	3.291	698	700	706	rVB	383	318	0.02%	0.003%
16	3.359	719	721	728	rVB3	521	337	0.02%	0.003%
17	3.474	753	757	761	rBV3	316	246	0.02%	0.002%
18	3.539	773	777	780	rBV2	251	240	0.02%	0.002%
19	3.674	816	819	821	rBV	257	199	0.01%	0.002%
20	3.751	839	843	845	rBV2	284	249	0.02%	0.002%
21	3.786	846	854	910	rVV	89477	270545	17.98%	2.416%
22	4.246	982	997	1033	rBV	232805	595987	39.60%	5.322%
23	4.484	1069	1071	1076	rBV4	593	350	0.02%	0.003%
24	4.677	1127	1131	1133	rBV3	681	483	0.03%	0.004%
25	4.744	1149	1152	1156	rBV2	790	601	0.04%	0.005%
26	4.796	1166	1168	1171	rVB3	534	303	0.02%	0.003%
27	4.838	1178	1181	1186	rBV4	596	452	0.03%	0.004%
28	4.957	1202	1218	1256	rVV2	568683	1505009	100.00%	13.439%
29	5.391	1349	1353	1356	rBV4	848	597	0.04%	0.005%
30	5.416	1359	1361	1368	rBV4	330	360	0.02%	0.003%
31	5.445	1368	1370	1373	rBV3	388	216	0.01%	0.002%
32	5.532	1386	1397	1436	rBV	404408	847744	56.33%	7.570%
33	5.834	1481	1491	1504	rBV6	6964	15290	1.02%	0.137%
34	5.928	1517	1520	1522	rBV2	590	339	0.02%	0.003%
35	5.944	1522	1525	1526	rBV	493	242	0.02%	0.002%
36	5.989	1526	1539	1572	rVV	326700	681252	45.27%	6.083%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034885.D
 Acq On : 28 Mar 2024 14:46
 Operator : SY/MD
 Sample : P1851-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.455	1682	1684	1689	rVB4	676	334	0.02%	0.003%
38	6.481	1690	1692	1698	rVB3	413	271	0.02%	0.002%
39	6.519	1702	1704	1706	rBV2	346	208	0.01%	0.002%
40	6.635	1737	1740	1742	rBV2	418	215	0.01%	0.002%
41	6.651	1742	1745	1746	rBV	313	202	0.01%	0.002%
42	6.661	1746	1748	1752	rVV3	572	438	0.03%	0.004%
43	6.683	1752	1755	1759	rVB2	407	265	0.02%	0.002%
44	6.725	1766	1768	1772	rVB2	348	244	0.02%	0.002%
45	6.754	1772	1777	1779	rBV	388	325	0.02%	0.003%
46	6.911	1816	1826	1849	rBV	164739	317381	21.09%	2.834%
47	7.243	1918	1929	1960	rBV	683058	1200120	79.74%	10.717%
48	7.551	2016	2025	2050	rBV	111077	210421	13.98%	1.879%
49	7.796	2097	2101	2102	rBV2	417	231	0.02%	0.002%
50	7.831	2109	2112	2116	rBV3	421	312	0.02%	0.003%
51	7.850	2116	2118	2119	rBV	486	210	0.01%	0.002%
52	7.985	2154	2160	2163	rBV3	346	379	0.03%	0.003%
53	8.024	2163	2172	2215	rBV	270522	594068	39.47%	5.305%
54	8.783	2396	2408	2443	rBV	641876	1064069	70.70%	9.502%
55	9.082	2500	2501	2504	rBV	437	255	0.02%	0.002%
56	9.149	2519	2522	2526	rBV4	390	271	0.02%	0.002%
57	9.349	2580	2584	2587	rBV3	537	463	0.03%	0.004%
58	9.419	2602	2606	2609	rBV	299	263	0.02%	0.002%
59	9.538	2640	2643	2645	rBV	355	244	0.02%	0.002%
60	9.612	2662	2666	2667	rBV2	355	228	0.02%	0.002%
61	9.792	2716	2722	2723	rBV	365	357	0.02%	0.003%
62	9.931	2761	2765	2769	rVV2	440	355	0.02%	0.003%
63	9.953	2769	2772	2776	rVB	356	213	0.01%	0.002%
64	10.011	2786	2790	2793	rVB2	442	328	0.02%	0.003%
65	10.053	2797	2803	2806	rBV2	591	556	0.04%	0.005%
66	10.152	2821	2834	2856	rBV	433558	699047	46.45%	6.242%
67	10.294	2876	2878	2882	rBV3	515	393	0.03%	0.004%
68	10.329	2882	2889	2895	rVB5	2555	3306	0.22%	0.030%
69	10.632	2981	2983	2987	rVB2	456	250	0.02%	0.002%
70	10.654	2987	2990	2992	rBV	498	311	0.02%	0.003%
71	10.689	3000	3001	3005	rVB	597	269	0.02%	0.002%
72	10.712	3005	3008	3010	rBV	617	315	0.02%	0.003%
73	10.744	3016	3018	3022	rVB2	442	263	0.02%	0.002%
74	10.767	3022	3025	3031	rBB3	515	409	0.03%	0.004%
75	10.863	3052	3055	3057	rBV2	388	209	0.01%	0.002%
76	10.934	3073	3077	3079	rBV	478	331	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034885.D
 Acq On : 28 Mar 2024 14:46
 Operator : SY/MD
 Sample : P1851-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.988	3090	3094	3097	rBV3	545	420	0.03%	0.004%
78	11.140	3131	3141	3144	rBV3	1034	1396	0.09%	0.012%
79	11.185	3144	3155	3177	rBV	648216	997223	66.26%	8.905%
80	11.558	3259	3271	3295	rBV	662160	1043246	69.32%	9.316%
81	11.792	3342	3344	3347	rBV2	381	252	0.02%	0.002%
82	11.937	3387	3389	3392	rVB2	466	217	0.01%	0.002%
83	12.037	3417	3420	3423	rBV2	688	496	0.03%	0.004%
84	12.185	3464	3466	3469	rBV2	485	314	0.02%	0.003%
85	12.233	3479	3481	3485	rBV3	319	233	0.02%	0.002%
86	12.278	3493	3495	3502	rVB3	438	386	0.03%	0.003%
87	12.307	3502	3504	3507	rBV2	280	199	0.01%	0.002%
88	12.342	3511	3515	3517	rBV2	709	589	0.04%	0.005%
89	12.567	3582	3585	3588	rBV2	522	354	0.02%	0.003%
90	12.683	3618	3621	3623	rBV3	509	270	0.02%	0.002%
91	12.767	3644	3647	3649	rBV	615	317	0.02%	0.003%
92	12.847	3668	3672	3676	rBV3	594	452	0.03%	0.004%
93	12.908	3688	3691	3694	rBV2	396	338	0.02%	0.003%
94	13.207	3782	3784	3791	rVB3	1820	1815	0.12%	0.016%
95	13.262	3796	3801	3803	rBV2	482	413	0.03%	0.004%
96	13.320	3815	3819	3822	rBV	453	330	0.02%	0.003%
97	13.410	3843	3847	3850	rBV2	391	292	0.02%	0.003%
98	13.451	3856	3860	3869	rVB4	2311	3114	0.21%	0.028%
99	13.580	3898	3900	3904	rBV3	465	291	0.02%	0.003%
100	13.853	3983	3985	3986	rBV3	470	206	0.01%	0.002%

Sum of corrected areas: 11198585




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034885.D
Acq On : 28 Mar 2024 14:46
Operator : SY/MD
Sample : P1851-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

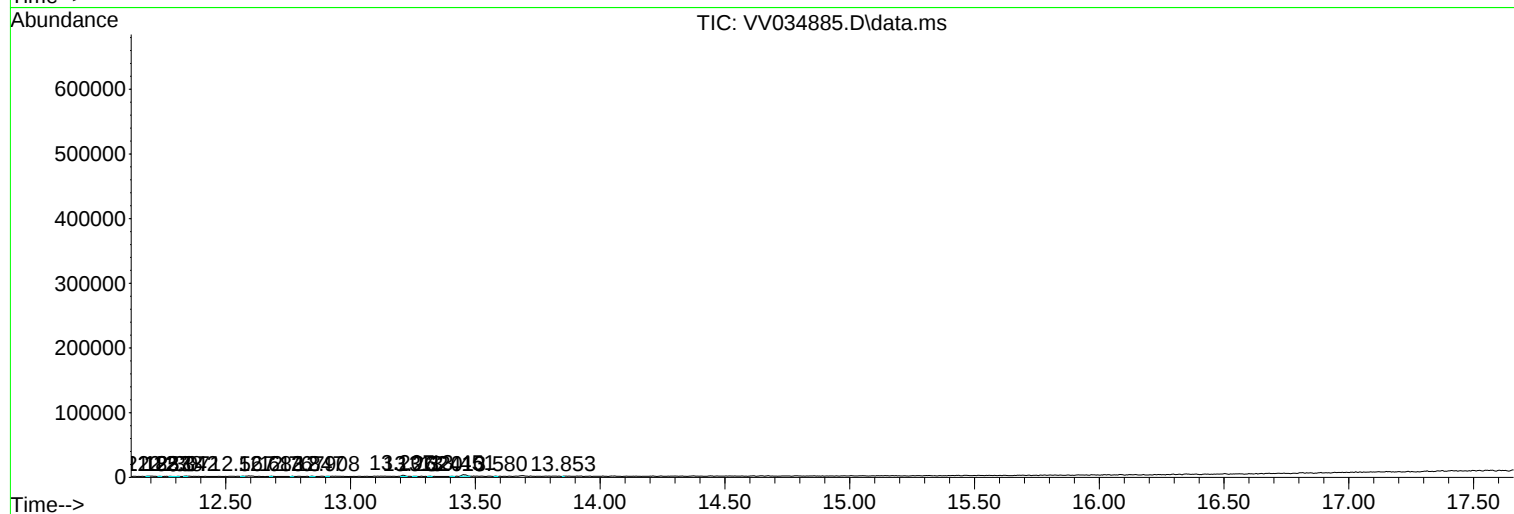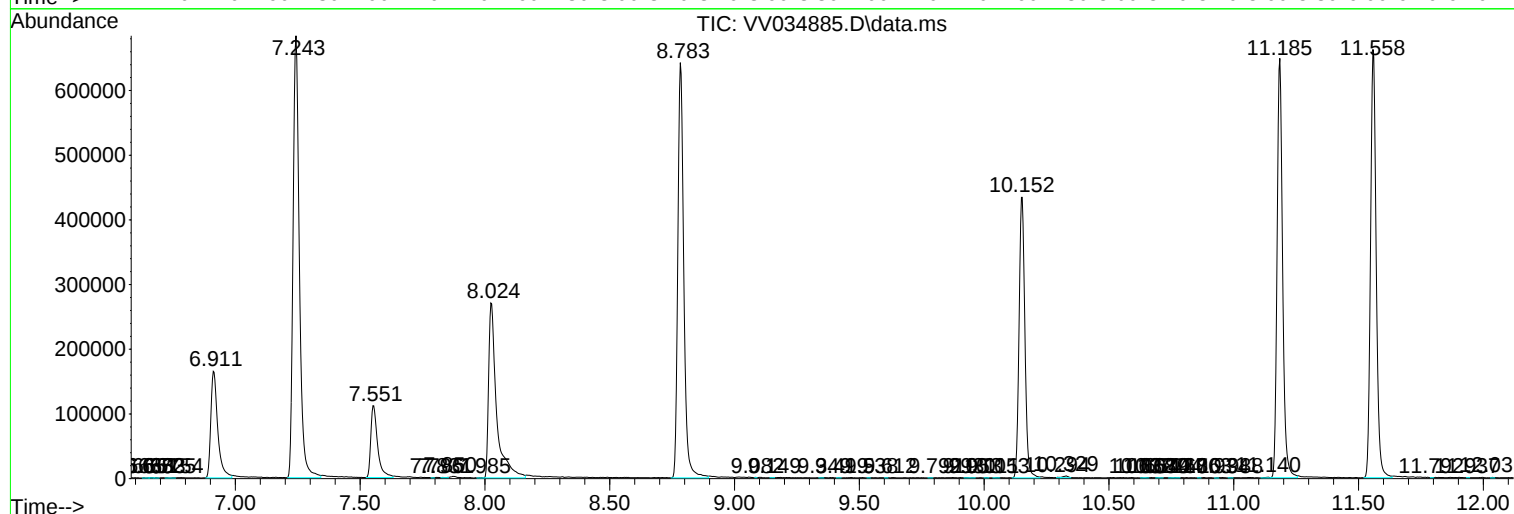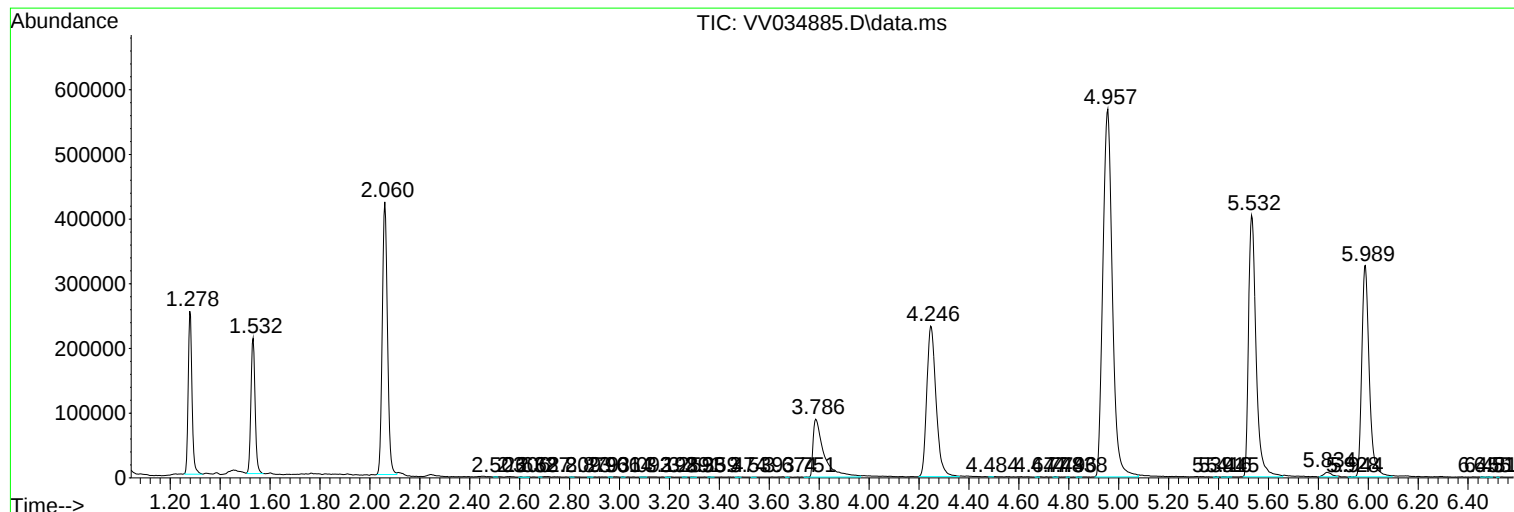

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034885.D
Acq On : 28 Mar 2024 14:46
Operator : SY/MD
Sample : P1851-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034885.D
Acq On : 28 Mar 2024 14:46
Operator : SY/MD
Sample : P1851-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
