

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034886.D
 Acq On : 28 Mar 2024 15:10
 Operator : SY/MD
 Sample : P1886-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	248576	259248	17.37%	2.331%
2	1.532	146	153	170	rVB	205420	245443	16.44%	2.206%
3	2.060	307	317	331	rBV	420059	608433	40.76%	5.470%
4	2.555	468	471	473	rBV	546	394	0.03%	0.004%
5	2.700	513	516	519	rVB3	336	256	0.02%	0.002%
6	2.748	527	531	535	rVB3	412	297	0.02%	0.003%
7	2.886	571	574	575	rBV3	650	397	0.03%	0.004%
8	2.963	594	598	602	rBV4	415	365	0.02%	0.003%
9	2.995	606	608	611	rBV2	297	170	0.01%	0.002%
10	3.124	646	648	651	rVB2	498	257	0.02%	0.002%
11	3.137	651	652	655	rVB2	384	174	0.01%	0.002%
12	3.163	655	660	661	rBV3	209	177	0.01%	0.002%
13	3.172	661	663	665	rBV	331	155	0.01%	0.001%
14	3.227	674	680	682	rBV	251	240	0.02%	0.002%
15	3.365	718	723	725	rBV2	304	254	0.02%	0.002%
16	3.384	727	729	732	rVV2	347	212	0.01%	0.002%
17	3.445	744	748	751	rBV2	475	324	0.02%	0.003%
18	3.465	752	754	757	rBV3	297	170	0.01%	0.002%
19	3.503	763	766	768	rBV2	307	193	0.01%	0.002%
20	3.555	777	782	783	rBV	238	202	0.01%	0.002%
21	3.584	787	791	793	rBV2	758	599	0.04%	0.005%
22	3.674	817	819	823	rBV3	257	179	0.01%	0.002%
23	3.728	834	836	840	rBV2	297	225	0.02%	0.002%
24	3.748	840	842	846	rBV2	380	279	0.02%	0.003%
25	3.786	846	854	896	rBV	88541	265670	17.80%	2.388%
26	4.246	983	997	1030	rBV	234150	644005	43.14%	5.789%
27	4.571	1096	1098	1101	rBV3	285	173	0.01%	0.002%
28	4.767	1157	1159	1160	rBV	358	177	0.01%	0.002%
29	4.815	1170	1174	1177	rBV2	341	286	0.02%	0.003%
30	4.953	1201	1217	1251	rBV2	564953	1492809	100.00%	13.420%
31	5.359	1341	1343	1345	rBV	599	306	0.02%	0.003%
32	5.436	1365	1367	1368	rBV2	306	164	0.01%	0.001%
33	5.471	1375	1378	1382	rBV2	666	675	0.05%	0.006%
34	5.532	1387	1397	1424	rBV	397652	822627	55.11%	7.395%
35	5.831	1481	1490	1508	rBV3	11760	26540	1.78%	0.239%
36	5.986	1526	1538	1568	rBV	318477	673816	45.14%	6.057%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034886.D
 Acq On : 28 Mar 2024 15:10
 Operator : SY/MD
 Sample : P1886-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.323	1640	1643	1645	rBV2	457	217	0.01%	0.002%
38	6.359	1651	1654	1655	rBV	648	319	0.02%	0.003%
39	6.387	1661	1663	1668	rVB2	572	427	0.03%	0.004%
40	6.445	1670	1681	1692	rBV2	5060	10307	0.69%	0.093%
41	6.555	1713	1715	1717	rBV2	426	224	0.02%	0.002%
42	6.568	1717	1719	1722	rVB	646	262	0.02%	0.002%
43	6.606	1725	1731	1732	rBV	333	289	0.02%	0.003%
44	6.751	1772	1776	1781	rBV4	618	657	0.04%	0.006%
45	6.809	1790	1794	1800	rBV3	383	415	0.03%	0.004%
46	6.912	1816	1826	1854	rVV	168164	319170	21.38%	2.869%
47	7.243	1918	1929	1950	rBV	669618	1183583	79.29%	10.640%
48	7.551	2016	2025	2055	rBV	112248	213346	14.29%	1.918%
49	7.834	2109	2113	2115	rBV3	567	530	0.04%	0.005%
50	7.953	2148	2150	2157	rVB3	396	398	0.03%	0.004%
51	7.995	2160	2163	2164	rBV2	642	425	0.03%	0.004%
52	8.024	2164	2172	2214	rBV2	274892	595631	39.90%	5.355%
53	8.339	2268	2270	2271	rBV	886	406	0.03%	0.004%
54	8.551	2332	2336	2339	rBV4	560	505	0.03%	0.005%
55	8.600	2348	2351	2353	rBV2	607	367	0.02%	0.003%
56	8.635	2360	2362	2364	rBV	336	202	0.01%	0.002%
57	8.725	2387	2390	2392	rBV2	497	268	0.02%	0.002%
58	8.783	2397	2408	2440	rBV	633423	1046445	70.10%	9.407%
59	9.079	2498	2500	2502	rBV2	595	267	0.02%	0.002%
60	9.169	2525	2528	2531	rBV3	468	283	0.02%	0.003%
61	9.243	2548	2551	2555	rBV2	354	326	0.02%	0.003%
62	9.268	2555	2559	2563	rVB2	638	433	0.03%	0.004%
63	9.291	2563	2566	2567	rBV2	301	182	0.01%	0.002%
64	9.448	2612	2615	2617	rBV2	353	168	0.01%	0.002%
65	9.574	2651	2654	2657	rVB2	442	303	0.02%	0.003%
66	9.622	2665	2669	2673	rBV2	500	409	0.03%	0.004%
67	9.654	2677	2679	2686	rVB4	684	573	0.04%	0.005%
68	9.866	2741	2745	2747	rBV3	457	335	0.02%	0.003%
69	9.895	2752	2754	2757	rBV2	425	285	0.02%	0.003%
70	9.947	2768	2770	2774	rBV2	346	261	0.02%	0.002%
71	10.005	2783	2788	2791	rBV3	329	339	0.02%	0.003%
72	10.072	2805	2809	2813	rBV4	360	356	0.02%	0.003%
73	10.153	2822	2834	2857	rBV	423343	680394	45.58%	6.117%
74	10.391	2902	2908	2911	rBV3	838	793	0.05%	0.007%
75	10.445	2923	2925	2929	rBV2	404	225	0.02%	0.002%
76	10.532	2950	2952	2954	rBV	549	320	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034886.D
 Acq On : 28 Mar 2024 15:10
 Operator : SY/MD
 Sample : P1886-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.593	2967	2971	2977	rBV2	232	200	0.01%	0.002%
78	10.622	2977	2980	2986	rBV3	390	407	0.03%	0.004%
79	10.648	2986	2988	2990	rBV	337	234	0.02%	0.002%
80	10.715	3007	3009	3010	rBV	499	219	0.01%	0.002%
81	10.857	3051	3053	3054	rBV	585	223	0.01%	0.002%
82	10.966	3085	3087	3091	rVB2	583	276	0.02%	0.002%
83	10.989	3091	3094	3097	rBV	375	256	0.02%	0.002%
84	11.034	3103	3108	3111	rBV2	282	319	0.02%	0.003%
85	11.069	3115	3119	3122	rBV2	487	356	0.02%	0.003%
86	11.185	3144	3155	3178	rBV	627159	975626	65.36%	8.771%
87	11.513	3252	3257	3258	rBV	504	438	0.03%	0.004%
88	11.558	3260	3271	3301	rVV	653568	1031607	69.11%	9.274%
89	11.931	3385	3387	3389	rBV	362	164	0.01%	0.001%
90	12.005	3408	3410	3415	rVB3	412	310	0.02%	0.003%
91	12.259	3487	3489	3493	rBV2	404	289	0.02%	0.003%
92	12.304	3498	3503	3504	rBV4	1010	816	0.05%	0.007%
93	12.407	3532	3535	3538	rBV	396	267	0.02%	0.002%
94	12.564	3582	3584	3588	rBV2	301	218	0.01%	0.002%
95	12.593	3588	3593	3599	rBV3	1182	1334	0.09%	0.012%
96	13.127	3757	3759	3763	rBV2	501	306	0.02%	0.003%
97	13.210	3778	3785	3793	rBV5	1603	2121	0.14%	0.019%
98	13.683	3929	3932	3933	rBV	1025	539	0.04%	0.005%
99	14.117	4065	4067	4070	rBV2	453	234	0.02%	0.002%
100	14.805	4279	4281	4284	rBV2	721	450	0.03%	0.004%




Sum of corrected areas: 11123745

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034886.D
Acq On : 28 Mar 2024 15:10
Operator : SY/MD
Sample : P1886-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

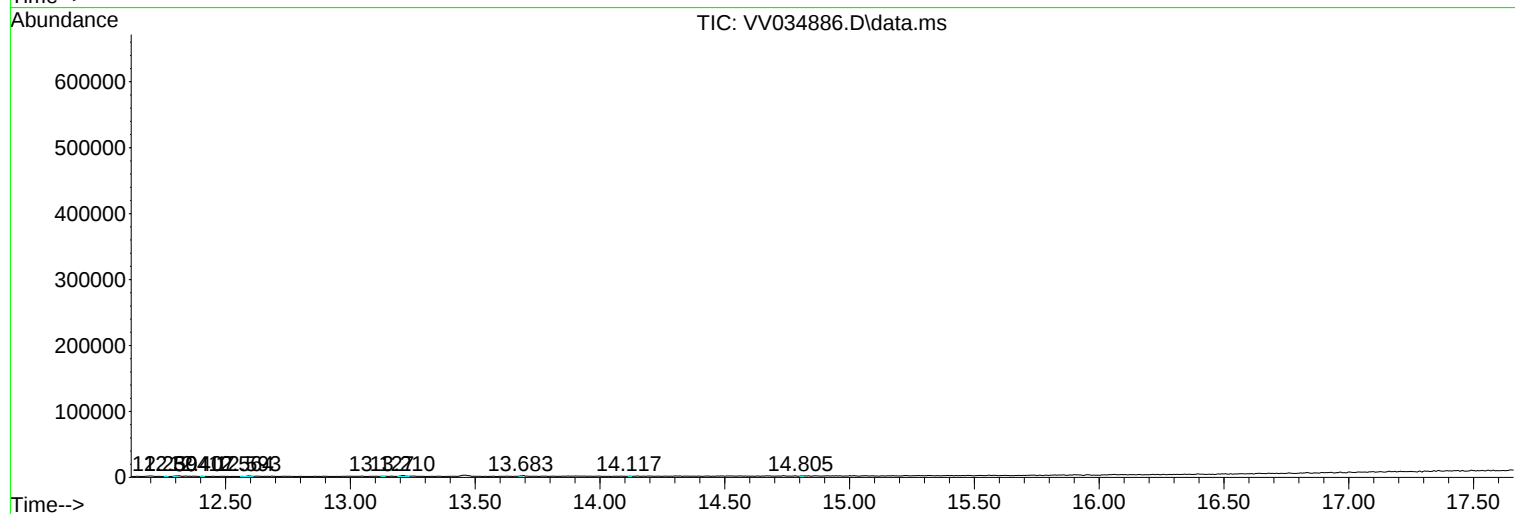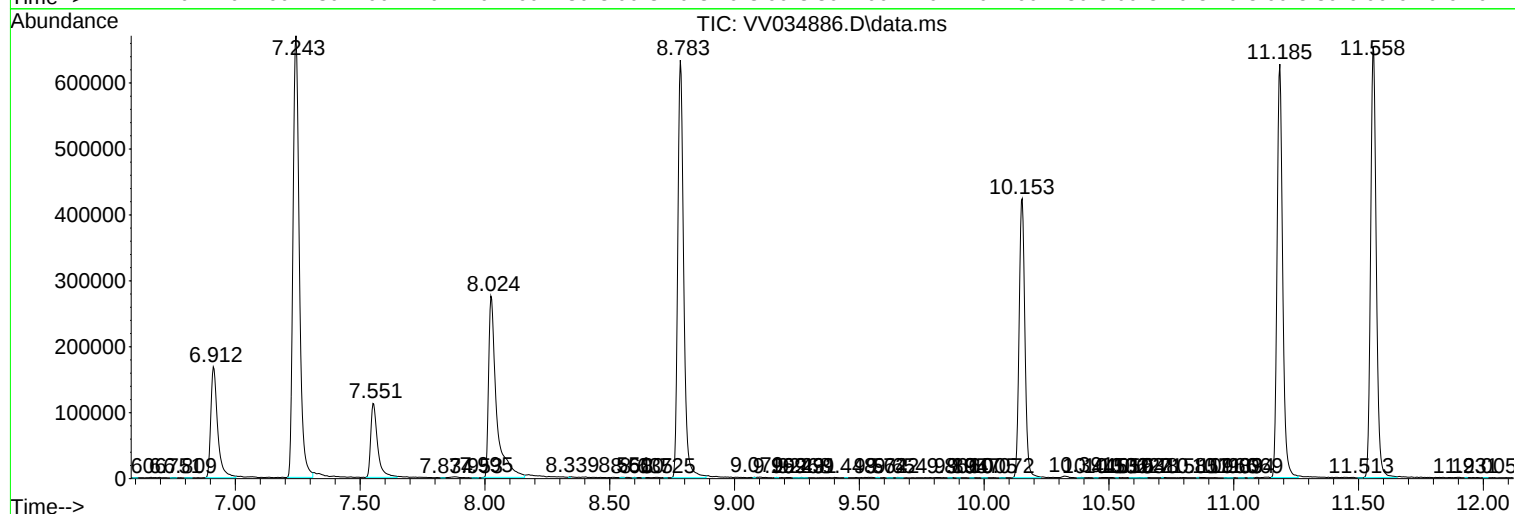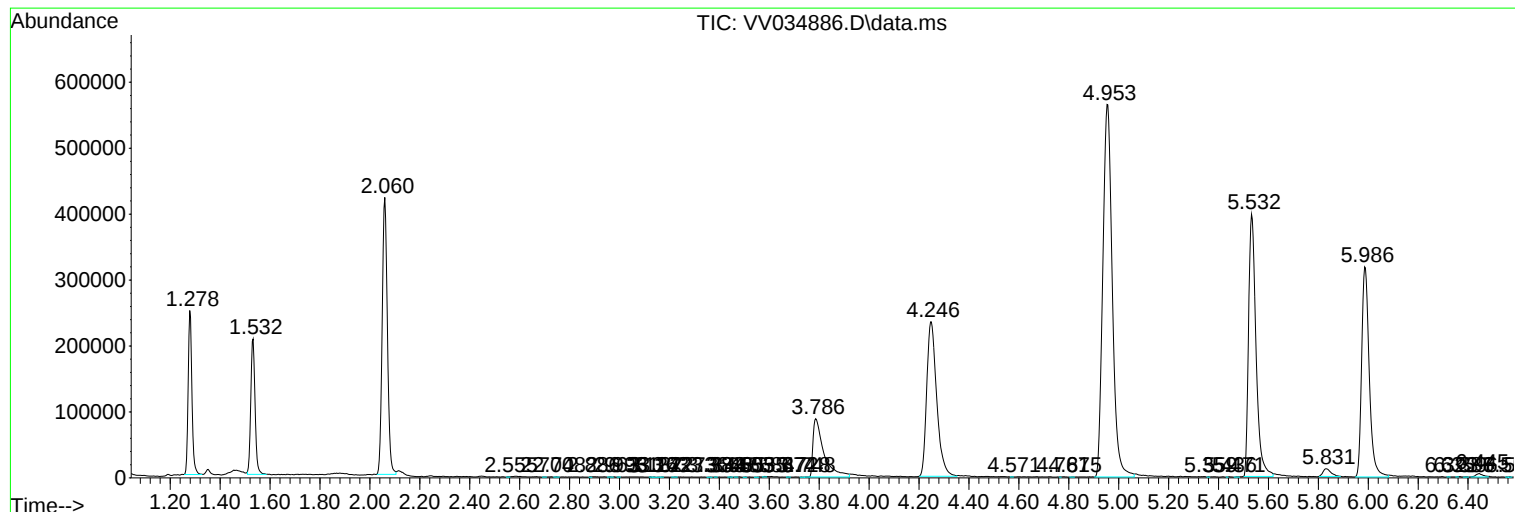

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034886.D
Acq On : 28 Mar 2024 15:10
Operator : SY/MD
Sample : P1886-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034886.D
Acq On : 28 Mar 2024 15:10
Operator : SY/MD
Sample : P1886-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc