

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034887.D
 Acq On : 28 Mar 2024 15:34
 Operator : SY/MD
 Sample : P1886-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	250111	265544	17.59%	2.370%
2	1.532	146	153	168	rVB	221669	259474	17.19%	2.316%
3	2.059	307	317	331	rBV	419975	609422	40.37%	5.439%
4	2.551	468	470	472	rBV2	311	178	0.01%	0.002%
5	2.568	472	475	478	rBV2	390	284	0.02%	0.003%
6	2.587	478	481	485	rBV2	677	498	0.03%	0.004%
7	2.715	516	521	523	rVV4	439	369	0.02%	0.003%
8	2.773	536	539	541	rBV2	504	283	0.02%	0.003%
9	2.953	591	595	599	rBV3	410	411	0.03%	0.004%
10	2.998	607	609	613	rVB	430	239	0.02%	0.002%
11	3.040	618	622	624	rBV4	338	253	0.02%	0.002%
12	3.076	630	633	636	rBV2	359	239	0.02%	0.002%
13	3.117	642	646	650	rBV3	326	280	0.02%	0.002%
14	3.204	670	673	675	rBV2	273	191	0.01%	0.002%
15	3.223	675	679	681	rBV	209	179	0.01%	0.002%
16	3.365	721	723	726	rBV	345	228	0.02%	0.002%
17	3.403	732	735	738	rBV3	358	266	0.02%	0.002%
18	3.436	742	745	747	rBV	333	228	0.02%	0.002%
19	3.558	778	783	786	rBV3	471	471	0.03%	0.004%
20	3.654	810	813	817	rVB4	469	360	0.02%	0.003%
21	3.754	841	844	847	rBV2	513	403	0.03%	0.004%
22	3.789	847	855	892	rBV	89777	264528	17.52%	2.361%
23	4.249	982	998	1029	rBV	237327	656022	43.46%	5.855%
24	4.561	1093	1095	1097	rBV	549	369	0.02%	0.003%
25	4.609	1105	1110	1115	rBV5	667	846	0.06%	0.008%
26	4.632	1115	1117	1118	rBV	437	195	0.01%	0.002%
27	4.741	1148	1151	1154	rVB2	720	415	0.03%	0.004%
28	4.764	1154	1158	1159	rBV3	519	317	0.02%	0.003%
29	4.956	1201	1218	1255	rBV2	566896	1509474	100.00%	13.473%
30	5.532	1386	1397	1428	rBV	403098	836400	55.41%	7.465%
31	5.831	1479	1490	1514	rBV3	13832	32668	2.16%	0.292%
32	5.989	1526	1539	1571	rBV	322645	673336	44.61%	6.010%
33	6.275	1624	1628	1630	rVB3	589	428	0.03%	0.004%
34	6.313	1638	1640	1643	rBV2	606	353	0.02%	0.003%
35	6.445	1671	1681	1692	rBV5	5919	11871	0.79%	0.106%
36	6.519	1702	1704	1706	rVB2	497	176	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034887.D
 Acq On : 28 Mar 2024 15:34
 Operator : SY/MD
 Sample : P1886-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.535	1706	1709	1711	rVB2	462	282	0.02%	0.003%
38	6.564	1714	1718	1720	rBV2	387	255	0.02%	0.002%
39	6.670	1748	1751	1753	rBV2	383	262	0.02%	0.002%
40	6.770	1780	1782	1783	rVV	376	173	0.01%	0.002%
41	6.821	1794	1798	1801	rBV2	312	225	0.01%	0.002%
42	6.911	1816	1826	1850	rBV2	165020	318775	21.12%	2.845%
43	7.124	1890	1892	1895	rBV3	440	249	0.02%	0.002%
44	7.243	1918	1929	1952	rBV	670064	1189571	78.81%	10.618%
45	7.554	2016	2026	2044	rBV	113461	207763	13.76%	1.854%
46	7.905	2133	2135	2138	rBV2	462	282	0.02%	0.003%
47	7.947	2145	2148	2152	rBV3	364	267	0.02%	0.002%
48	8.027	2164	2173	2212	rVV2	276391	602604	39.92%	5.379%
49	8.696	2375	2381	2390	rVB4	645	1005	0.07%	0.009%
50	8.738	2390	2394	2396	rVB2	522	349	0.02%	0.003%
51	8.783	2396	2408	2432	rBV	627340	1044815	69.22%	9.326%
52	9.027	2481	2484	2486	rBV2	838	506	0.03%	0.005%
53	9.085	2500	2502	2503	rBV	399	164	0.01%	0.001%
54	9.127	2513	2515	2516	rBV2	421	166	0.01%	0.001%
55	9.191	2531	2535	2538	rVB5	798	684	0.05%	0.006%
56	9.230	2544	2547	2548	rBV	428	196	0.01%	0.002%
57	9.249	2551	2553	2559	rVB3	431	370	0.02%	0.003%
58	9.448	2613	2615	2620	rVB3	322	223	0.01%	0.002%
59	9.567	2651	2652	2655	rVB3	547	238	0.02%	0.002%
60	9.638	2672	2674	2676	rBV	276	168	0.01%	0.001%
61	9.651	2676	2678	2680	rVV	367	171	0.01%	0.002%
62	9.696	2686	2692	2695	rBV2	770	667	0.04%	0.006%
63	9.734	2701	2704	2706	rBV2	358	201	0.01%	0.002%
64	9.799	2720	2724	2727	rBV2	609	528	0.03%	0.005%
65	9.841	2735	2737	2741	rBV2	331	227	0.02%	0.002%
66	9.908	2755	2758	2761	rVB2	646	328	0.02%	0.003%
67	9.937	2762	2767	2770	rVB3	415	313	0.02%	0.003%
68	9.966	2775	2776	2781	rBV3	582	458	0.03%	0.004%
69	10.033	2792	2797	2799	rBV2	566	427	0.03%	0.004%
70	10.152	2822	2834	2855	rBV	428353	678013	44.92%	6.052%
71	10.326	2879	2888	2900	rBV7	2002	3687	0.24%	0.033%
72	10.461	2928	2930	2933	rBV2	325	224	0.01%	0.002%
73	10.487	2935	2938	2942	rVB2	488	323	0.02%	0.003%
74	10.506	2942	2944	2946	rBV	341	217	0.01%	0.002%
75	10.561	2959	2961	2966	rVB3	470	277	0.02%	0.002%
76	10.590	2966	2970	2975	rBV2	438	417	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034887.D
 Acq On : 28 Mar 2024 15:34
 Operator : SY/MD
 Sample : P1886-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.689	2999	3001	3003	rBV2	463	185	0.01%	0.002%
78	10.747	3017	3019	3025	rVB3	329	296	0.02%	0.003%
79	10.863	3050	3055	3061	rBV3	602	796	0.05%	0.007%
80	10.924	3069	3074	3077	rVB2	901	658	0.04%	0.006%
81	10.943	3077	3080	3083	rBV2	384	261	0.02%	0.002%
82	10.969	3083	3088	3091	rBV2	569	417	0.03%	0.004%
83	11.030	3104	3107	3110	rBV2	408	245	0.02%	0.002%
84	11.185	3143	3155	3181	rBV	628491	979378	64.88%	8.741%
85	11.558	3258	3271	3292	rBV	645090	1031388	68.33%	9.206%
86	11.869	3366	3368	3371	rBV	321	220	0.01%	0.002%
87	11.953	3391	3394	3396	rBV3	421	253	0.02%	0.002%
88	12.127	3446	3448	3451	rBV2	375	212	0.01%	0.002%
89	12.194	3467	3469	3471	rBV2	412	213	0.01%	0.002%
90	12.310	3501	3505	3507	rBV3	1161	831	0.06%	0.007%
91	12.371	3521	3524	3526	rBV3	479	256	0.02%	0.002%
92	12.474	3552	3556	3558	rBV2	461	334	0.02%	0.003%
93	12.548	3577	3579	3582	rVB2	481	234	0.02%	0.002%
94	12.593	3587	3593	3597	rBV6	966	982	0.07%	0.009%
95	12.754	3642	3643	3646	rVB2	385	205	0.01%	0.002%
96	12.873	3677	3680	3684	rBV3	494	348	0.02%	0.003%
97	12.918	3692	3694	3699	rBV3	372	263	0.02%	0.002%
98	13.217	3778	3787	3794	rBV5	1161	2034	0.13%	0.018%
99	13.410	3845	3847	3850	rBV2	445	206	0.01%	0.002%
100	13.731	3945	3947	3950	rBV2	469	300	0.02%	0.003%




Sum of corrected areas: 11203783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034887.D
Acq On : 28 Mar 2024 15:34
Operator : SY/MD
Sample : P1886-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

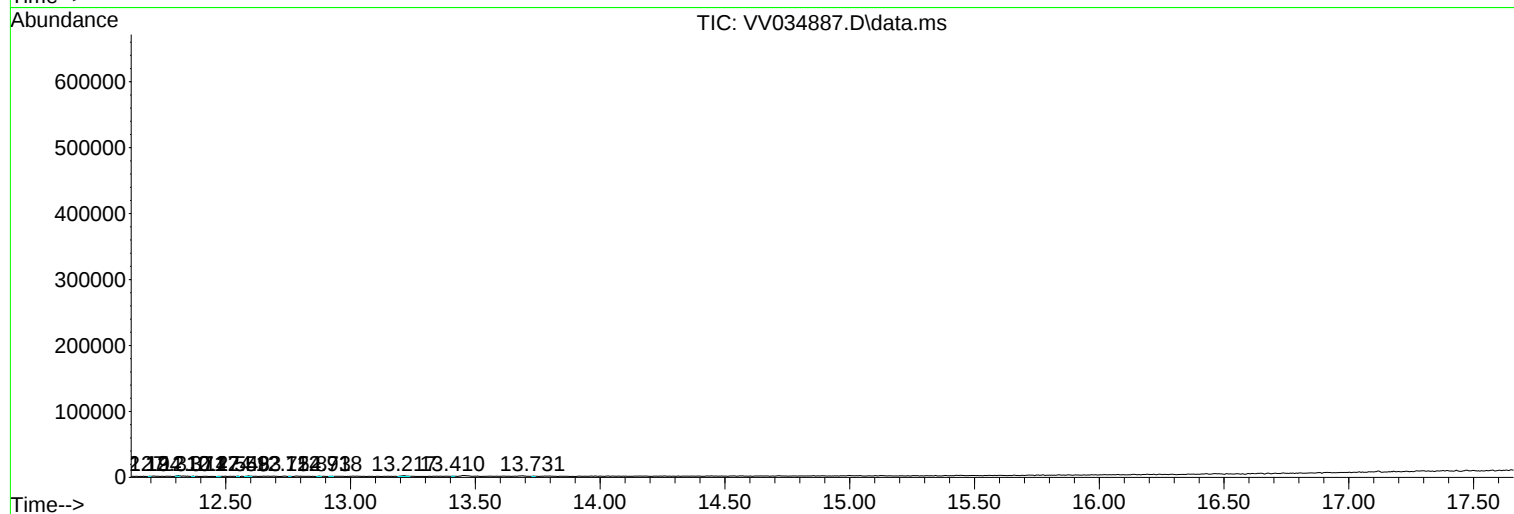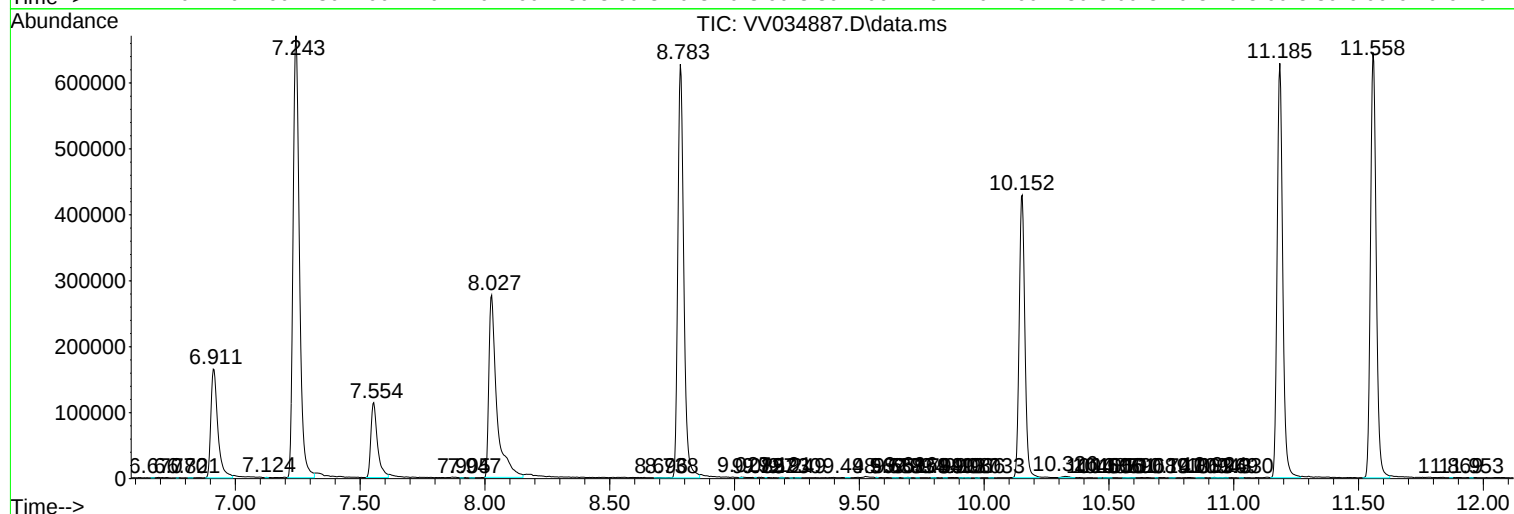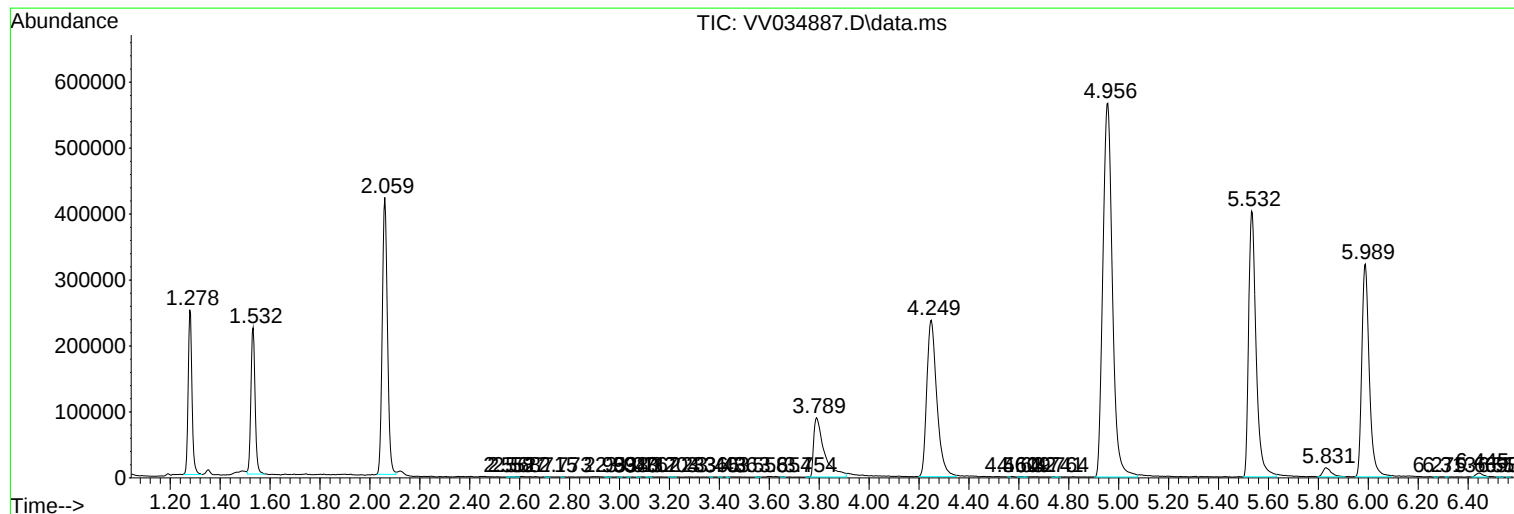

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034887.D
Acq On : 28 Mar 2024 15:34
Operator : SY/MD
Sample : P1886-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034887.D
Acq On : 28 Mar 2024 15:34
Operator : SY/MD
Sample : P1886-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc