

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034888.D
 Acq On : 28 Mar 2024 15:58
 Operator : SY/MD
 Sample : P1822-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0778

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rBV	220699	232912	16.87%	2.186%
2	1.532	146	153	169	rVB	206650	243111	17.60%	2.282%
3	2.060	307	317	331	rBV	375145	543405	39.35%	5.101%
4	2.439	433	435	440	rBV5	770	815	0.06%	0.008%
5	2.539	463	466	467	rBV5	440	200	0.01%	0.002%
6	2.568	474	475	477	rBV	281	116	0.01%	0.001%
7	2.584	477	480	484	rBV3	585	608	0.04%	0.006%
8	2.725	521	524	526	rBV2	470	222	0.02%	0.002%
9	2.738	526	528	531	rVB	443	200	0.01%	0.002%
10	2.757	531	534	537	rBV2	397	281	0.02%	0.003%
11	2.834	554	558	559	rBV	372	235	0.02%	0.002%
12	3.002	607	610	614	rBV2	167	100	0.01%	0.001%
13	3.137	649	652	655	rVB	334	223	0.02%	0.002%
14	3.153	655	657	659	rBV	438	292	0.02%	0.003%
15	3.265	689	692	694	rBV	261	195	0.01%	0.002%
16	3.291	697	700	702	rVB2	284	138	0.01%	0.001%
17	3.310	702	706	707	rBV3	271	190	0.01%	0.002%
18	3.416	736	739	741	rBV2	516	229	0.02%	0.002%
19	3.555	780	782	786	rVB2	400	195	0.01%	0.002%
20	3.654	810	813	816	rBV2	309	225	0.02%	0.002%
21	3.719	831	833	835	rBV2	168	99	0.01%	0.001%
22	3.744	838	841	846	rBV2	400	295	0.02%	0.003%
23	3.793	847	856	891	rBV	78934	237896	17.23%	2.233%
24	4.249	983	998	1030	rBV	216453	600343	43.47%	5.635%
25	4.677	1127	1131	1135	rBV3	431	400	0.03%	0.004%
26	4.732	1146	1148	1149	rBV	447	184	0.01%	0.002%
27	4.764	1155	1158	1162	rBV2	695	426	0.03%	0.004%
28	4.957	1201	1218	1253	rBV2	522546	1381023	100.00%	12.963%
29	5.365	1343	1345	1346	rBV2	391	154	0.01%	0.001%
30	5.532	1386	1397	1430	rBV	412714	859173	62.21%	8.064%
31	5.831	1480	1490	1504	rBV4	13046	27354	1.98%	0.257%
32	5.989	1526	1539	1562	rBV	300642	624468	45.22%	5.861%
33	6.256	1620	1622	1624	rBV2	542	288	0.02%	0.003%
34	6.297	1632	1635	1638	rBV	696	531	0.04%	0.005%
35	6.407	1666	1669	1670	rBV	563	271	0.02%	0.003%
36	6.442	1670	1680	1691	rVV5	4395	8715	0.63%	0.082%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034888.D
 Acq On : 28 Mar 2024 15:58
 Operator : SY/MD
 Sample : P1822-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0778

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.542	1707	1711	1712	rBV3	282	158	0.01%	0.001%
38	6.567	1717	1719	1720	rBV	416	160	0.01%	0.002%
39	6.645	1738	1743	1744	rBV2	329	280	0.02%	0.003%
40	6.715	1761	1765	1767	rBV	485	379	0.03%	0.004%
41	6.754	1776	1777	1780	rVB2	527	219	0.02%	0.002%
42	6.770	1780	1782	1783	rBV	356	153	0.01%	0.001%
43	6.796	1788	1790	1793	rVV2	310	170	0.01%	0.002%
44	6.911	1816	1826	1857	rBV	153225	299603	21.69%	2.812%
45	7.198	1913	1915	1918	rBV2	529	306	0.02%	0.003%
46	7.243	1918	1929	1953	rBV	624918	1092875	79.14%	10.258%
47	7.555	2016	2026	2055	rBV	103071	200437	14.51%	1.881%
48	7.866	2117	2123	2128	rBV4	986	1208	0.09%	0.011%
49	7.934	2141	2144	2145	rBV3	396	162	0.01%	0.002%
50	7.944	2145	2147	2151	rVB2	419	212	0.02%	0.002%
51	7.966	2151	2154	2157	rBV2	429	250	0.02%	0.002%
52	7.989	2157	2161	2164	rBV3	603	556	0.04%	0.005%
53	8.027	2164	2173	2209	rBV2	251438	558371	40.43%	5.241%
54	8.481	2312	2314	2315	rBV	470	127	0.01%	0.001%
55	8.735	2388	2393	2396	rBV2	316	322	0.02%	0.003%
56	8.783	2397	2408	2441	rBV	646903	1085164	78.58%	10.186%
57	9.198	2534	2537	2538	rBV	375	195	0.01%	0.002%
58	9.455	2615	2617	2620	rBV2	485	257	0.02%	0.002%
59	9.545	2642	2645	2646	rBV2	563	329	0.02%	0.003%
60	9.709	2693	2696	2699	rBV2	327	219	0.02%	0.002%
61	9.757	2709	2711	2715	rBV2	511	308	0.02%	0.003%
62	9.776	2715	2717	2721	rBV3	514	415	0.03%	0.004%
63	9.812	2725	2728	2729	rBV	324	158	0.01%	0.001%
64	9.963	2771	2775	2778	rBV2	590	537	0.04%	0.005%
65	10.017	2790	2792	2793	rBV	216	112	0.01%	0.001%
66	10.111	2819	2821	2822	rBV	248	102	0.01%	0.001%
67	10.153	2822	2834	2854	rVV	401035	634685	45.96%	5.957%
68	10.362	2896	2899	2901	rBV	491	271	0.02%	0.003%
69	10.387	2904	2907	2909	rBV2	218	152	0.01%	0.001%
70	10.439	2921	2923	2924	rBV2	289	104	0.01%	0.001%
71	10.606	2972	2975	2980	rVB2	430	330	0.02%	0.003%
72	10.767	3020	3025	3026	rBV	324	260	0.02%	0.002%
73	10.915	3069	3071	3073	rBV	564	327	0.02%	0.003%
74	11.001	3096	3098	3099	rBV	472	193	0.01%	0.002%
75	11.124	3133	3136	3141	rVB4	725	641	0.05%	0.006%
76	11.185	3141	3155	3183	rBV	648228	1025499	74.26%	9.626%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034888.D
 Acq On : 28 Mar 2024 15:58
 Operator : SY/MD
 Sample : P1822-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0778

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.435	3231	3233	3237	rBV2	495	317	0.02%	0.003%
78	11.516	3256	3258	3260	rBV2	779	442	0.03%	0.004%
79	11.558	3260	3271	3298	rVV	603674	972585	70.42%	9.129%
80	11.808	3347	3349	3352	rVB3	489	262	0.02%	0.002%
81	11.847	3357	3361	3362	rBV	361	253	0.02%	0.002%
82	11.902	3376	3378	3382	rVB2	560	262	0.02%	0.002%
83	11.937	3387	3389	3392	rVV3	728	372	0.03%	0.003%
84	11.956	3392	3395	3399	rVB2	507	353	0.03%	0.003%
85	12.008	3408	3411	3415	rBV3	600	499	0.04%	0.005%
86	12.072	3430	3431	3435	rVB2	369	189	0.01%	0.002%
87	12.111	3441	3443	3445	rBV	384	213	0.02%	0.002%
88	12.175	3460	3463	3466	rBV	689	525	0.04%	0.005%
89	12.242	3482	3484	3492	rVB3	550	549	0.04%	0.005%
90	12.275	3492	3494	3496	rBV	308	149	0.01%	0.001%
91	12.406	3533	3535	3539	rBV2	455	258	0.02%	0.002%
92	12.519	3566	3570	3573	rBV3	580	566	0.04%	0.005%
93	12.593	3589	3593	3597	rVB5	808	649	0.05%	0.006%
94	12.995	3714	3718	3721	rBV3	543	514	0.04%	0.005%
95	13.101	3749	3751	3760	rVB4	695	577	0.04%	0.005%
96	13.162	3768	3770	3773	rVB	501	186	0.01%	0.002%
97	13.213	3780	3786	3792	rBV6	1046	1443	0.10%	0.014%
98	13.300	3811	3813	3816	rBV2	387	148	0.01%	0.001%
99	13.422	3848	3851	3854	rBV	550	410	0.03%	0.004%
100	13.795	3964	3967	3971	rBV3	687	476	0.03%	0.004%




Sum of corrected areas: 10653915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034888.D
Acq On : 28 Mar 2024 15:58
Operator : SY/MD
Sample : P1822-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0778

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

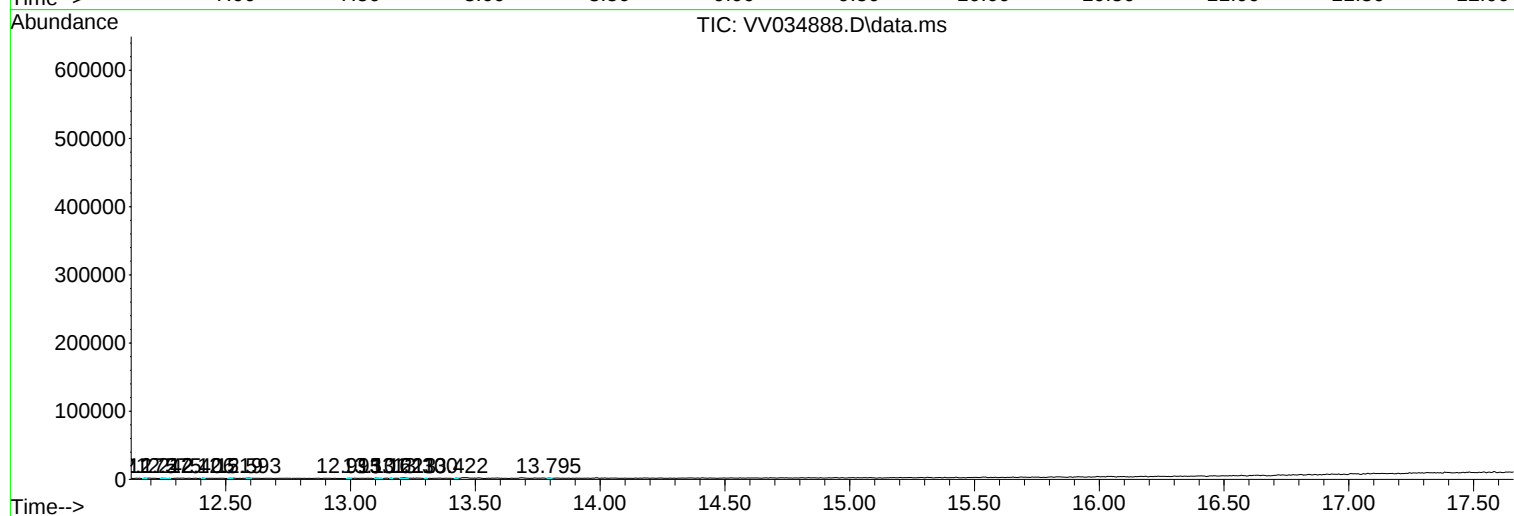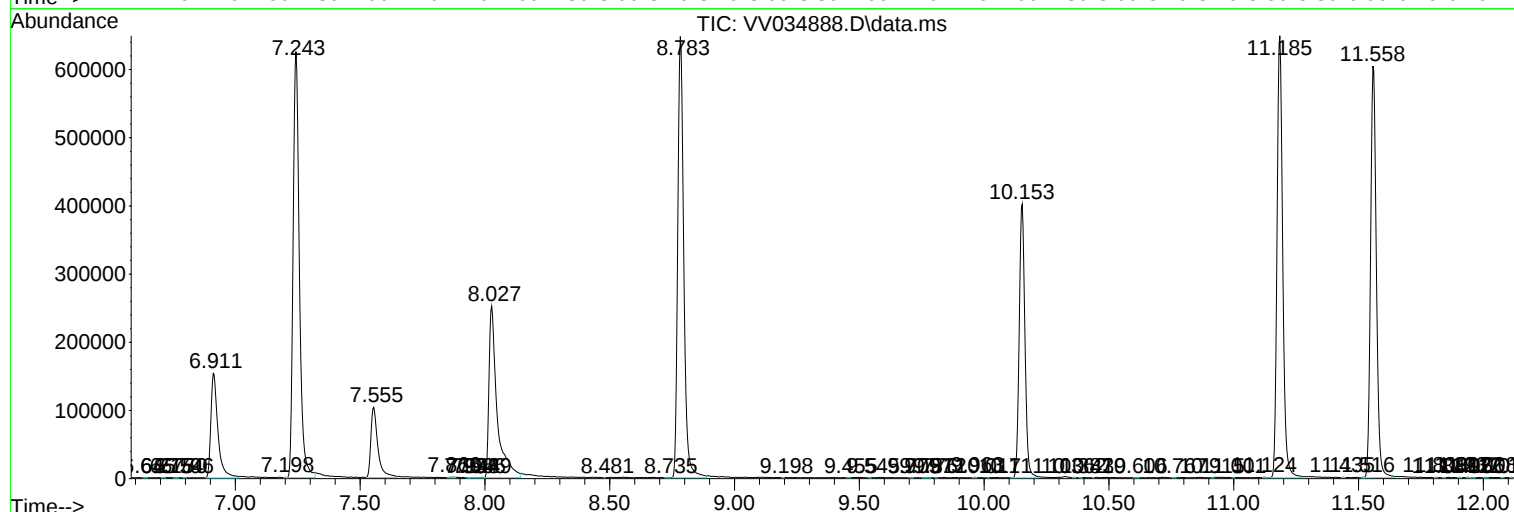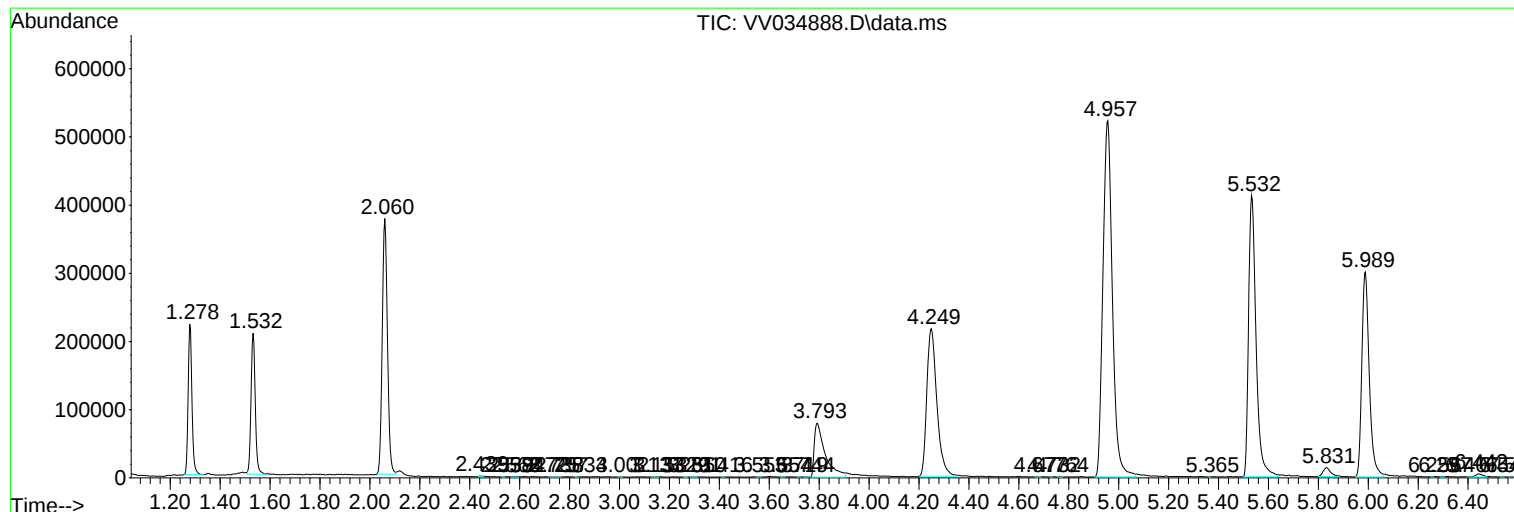

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034888.D
Acq On : 28 Mar 2024 15:58
Operator : SY/MD
Sample : P1822-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0778

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034888.D
Acq On : 28 Mar 2024 15:58
Operator : SY/MD
Sample : P1822-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0778

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------