

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034889.D
 Acq On : 28 Mar 2024 16:22
 Operator : SY/MD
 Sample : P1822-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	222149	233677	16.63%	2.137%
2	1.532	146	153	169	rVB	202550	237102	16.88%	2.168%
3	2.059	307	317	331	rBV	375613	543636	38.70%	4.971%
4	2.744	529	530	534	rVB2	304	173	0.01%	0.002%
5	2.767	534	537	539	rBV2	504	345	0.02%	0.003%
6	2.860	563	566	568	rBV	373	217	0.02%	0.002%
7	2.886	572	574	575	rBV	377	172	0.01%	0.002%
8	3.011	610	613	614	rBV	256	133	0.01%	0.001%
9	3.063	626	629	630	rBV2	388	199	0.01%	0.002%
10	3.114	641	645	647	rBV3	367	252	0.02%	0.002%
11	3.124	647	648	655	rVB3	269	173	0.01%	0.002%
12	3.172	659	663	664	rBV	433	364	0.03%	0.003%
13	3.252	685	688	691	rBV2	253	212	0.02%	0.002%
14	3.278	691	696	698	rVV3	443	348	0.02%	0.003%
15	3.326	707	711	714	rBV2	526	295	0.02%	0.003%
16	3.346	715	717	722	rVB3	247	164	0.01%	0.001%
17	3.381	722	728	729	rBV2	251	247	0.02%	0.002%
18	3.497	762	764	769	rBV2	239	137	0.01%	0.001%
19	3.519	769	771	773	rBV	215	118	0.01%	0.001%
20	3.545	777	779	781	rBV	314	141	0.01%	0.001%
21	3.571	784	787	789	rBV	232	141	0.01%	0.001%
22	3.600	793	796	797	rBV	673	433	0.03%	0.004%
23	3.706	827	829	834	rVB2	552	374	0.03%	0.003%
24	3.735	834	838	839	rBV2	432	313	0.02%	0.003%
25	3.789	847	855	897	rBV2	84522	259444	18.47%	2.372%
26	4.249	982	998	1028	rBV	227028	629968	44.84%	5.760%
27	4.612	1108	1111	1116	rVB3	615	448	0.03%	0.004%
28	4.690	1131	1135	1139	rBV3	451	450	0.03%	0.004%
29	4.712	1139	1142	1145	rVB3	479	283	0.02%	0.003%
30	4.741	1145	1151	1153	rBV3	413	404	0.03%	0.004%
31	4.767	1156	1159	1161	rBV2	491	354	0.03%	0.003%
32	4.809	1170	1172	1175	rBV3	377	259	0.02%	0.002%
33	4.956	1202	1218	1249	rBV2	536344	1404860	100.00%	12.846%
34	5.326	1331	1333	1335	rBV3	511	273	0.02%	0.002%
35	5.474	1374	1379	1384	rBV3	621	548	0.04%	0.005%
36	5.532	1384	1397	1434	rBV	426624	890169	63.36%	8.140%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034889.D
 Acq On : 28 Mar 2024 16:22
 Operator : SY/MD
 Sample : P1822-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.831	1481	1490	1503	rBV2	12068	26205	1.87%	0.240%
38	5.989	1525	1539	1567	rBV	310384	639351	45.51%	5.846%
39	6.278	1626	1629	1636	rVB4	808	903	0.06%	0.008%
40	6.307	1636	1638	1642	rBV2	200	151	0.01%	0.001%
41	6.445	1675	1681	1696	rVB4	4784	9944	0.71%	0.091%
42	6.577	1720	1722	1725	rVB	234	120	0.01%	0.001%
43	6.593	1725	1727	1729	rBV	485	241	0.02%	0.002%
44	6.606	1729	1731	1733	rVV2	368	203	0.01%	0.002%
45	6.657	1743	1747	1750	rBV3	382	330	0.02%	0.003%
46	6.693	1756	1758	1761	rBV	314	192	0.01%	0.002%
47	6.744	1772	1774	1778	rBV2	471	208	0.01%	0.002%
48	6.796	1787	1790	1792	rBV2	289	197	0.01%	0.002%
49	6.834	1799	1802	1805	rBV2	259	174	0.01%	0.002%
50	6.915	1813	1827	1859	rBV	158319	309889	22.06%	2.834%
51	7.243	1918	1929	1951	rBV	630727	1108432	78.90%	10.136%
52	7.554	2017	2026	2051	rBV	106551	199906	14.23%	1.828%
53	7.841	2113	2115	2117	rBV2	643	396	0.03%	0.004%
54	7.873	2121	2125	2130	rVV4	739	780	0.06%	0.007%
55	7.918	2138	2139	2142	rBV2	384	165	0.01%	0.002%
56	7.992	2160	2162	2164	rBV3	452	211	0.02%	0.002%
57	8.027	2164	2173	2213	rBV2	267528	584721	41.62%	5.347%
58	8.599	2349	2351	2356	rVB2	726	551	0.04%	0.005%
59	8.632	2358	2361	2364	rBV2	682	411	0.03%	0.004%
60	8.712	2382	2386	2387	rBV2	335	226	0.02%	0.002%
61	8.783	2397	2408	2440	rBV	677430	1121597	79.84%	10.256%
62	9.091	2501	2504	2505	rBV4	569	340	0.02%	0.003%
63	9.329	2574	2578	2581	rBV3	501	412	0.03%	0.004%
64	9.410	2602	2603	2604	rBV3	196	59	0.00%	0.001%
65	9.468	2619	2621	2628	rBV2	324	304	0.02%	0.003%
66	9.577	2651	2655	2657	rBV	499	384	0.03%	0.004%
67	9.664	2680	2682	2690	rVB2	513	478	0.03%	0.004%
68	9.699	2690	2693	2694	rBV2	367	180	0.01%	0.002%
69	9.802	2722	2725	2729	rBV2	519	415	0.03%	0.004%
70	9.918	2758	2761	2762	rBV	459	260	0.02%	0.002%
71	9.953	2769	2772	2775	rBV2	489	339	0.02%	0.003%
72	9.969	2775	2777	2779	rVV	416	185	0.01%	0.002%
73	9.988	2781	2783	2784	rVV	529	212	0.02%	0.002%
74	10.011	2788	2790	2796	rVB3	512	296	0.02%	0.003%
75	10.037	2796	2798	2800	rBV	371	196	0.01%	0.002%
76	10.152	2822	2834	2861	rBV	416233	655137	46.63%	5.991%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034889.D
 Acq On : 28 Mar 2024 16:22
 Operator : SY/MD
 Sample : P1822-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.448	2922	2926	2928	rBV2	344	313	0.02%	0.003%
78	10.506	2942	2944	2947	rBV	322	194	0.01%	0.002%
79	10.686	2997	3000	3003	rBV	254	198	0.01%	0.002%
80	10.705	3003	3006	3007	rBV	666	333	0.02%	0.003%
81	10.770	3024	3026	3028	rBV2	318	135	0.01%	0.001%
82	10.795	3032	3034	3036	rBV	311	202	0.01%	0.002%
83	11.136	3138	3140	3144	rVB3	848	538	0.04%	0.005%
84	11.184	3144	3155	3181	rBV	678390	1060318	75.47%	9.696%
85	11.557	3259	3271	3299	rBV	623276	998378	71.07%	9.129%
86	11.972	3398	3400	3406	rVB3	478	350	0.02%	0.003%
87	12.152	3453	3456	3463	rBV2	569	663	0.05%	0.006%
88	12.220	3474	3477	3479	rBV2	402	207	0.01%	0.002%
89	12.233	3479	3481	3482	rBV	452	179	0.01%	0.002%
90	12.287	3493	3498	3499	rBV	633	462	0.03%	0.004%
91	12.339	3511	3514	3515	rBV	515	314	0.02%	0.003%
92	12.480	3555	3558	3561	rBV	461	337	0.02%	0.003%
93	12.763	3645	3646	3651	rBV3	547	331	0.02%	0.003%
94	12.898	3683	3688	3690	rBV3	628	583	0.04%	0.005%
95	12.946	3701	3703	3704	rBV	404	145	0.01%	0.001%
96	13.869	3988	3990	3991	rBV	494	184	0.01%	0.002%
97	13.972	4020	4022	4025	rBV3	407	243	0.02%	0.002%




Sum of corrected areas: 10936134

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034889.D
Acq On : 28 Mar 2024 16:22
Operator : SY/MD
Sample : P1822-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0786

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

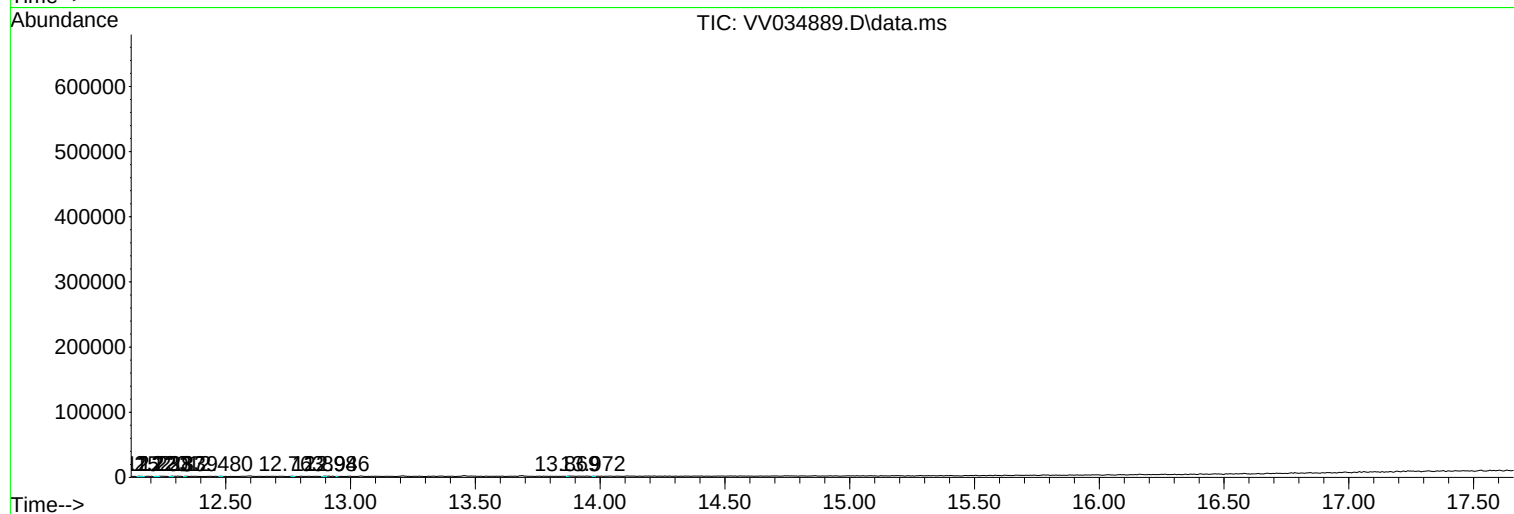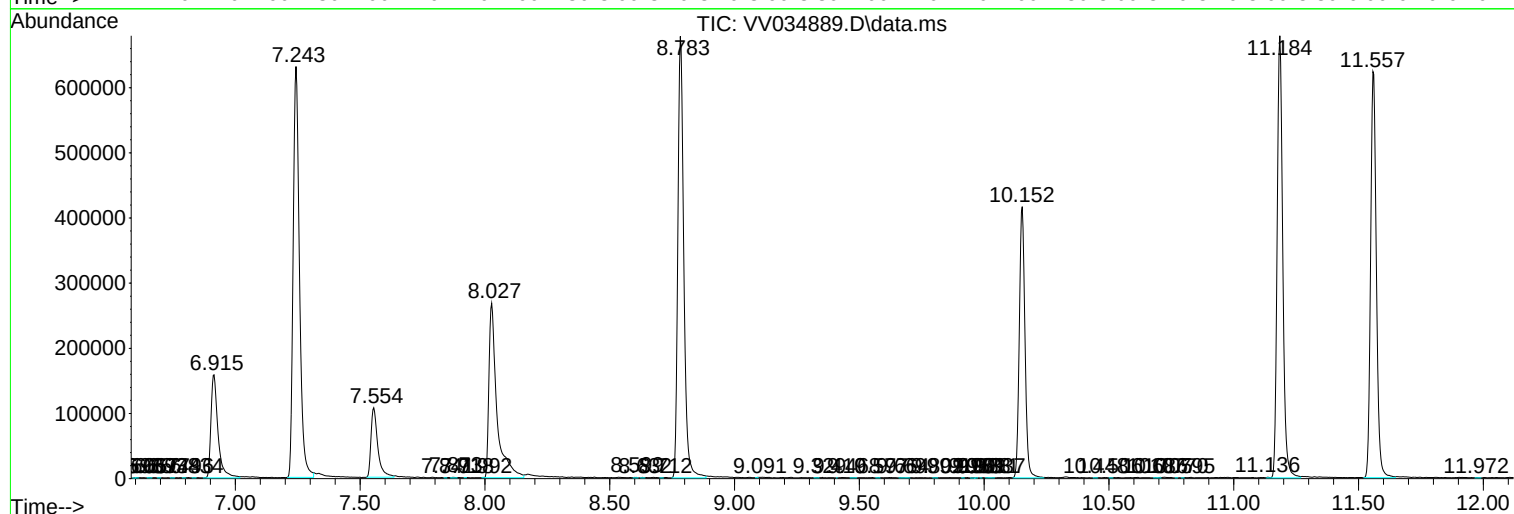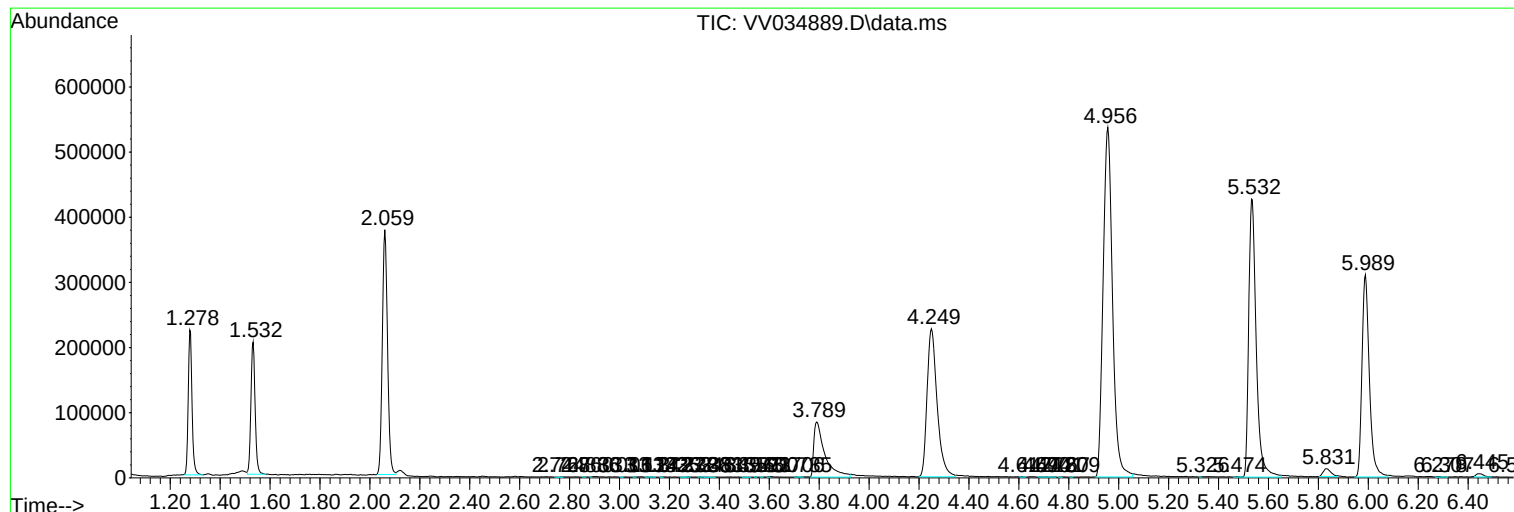

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034889.D
Acq On : 28 Mar 2024 16:22
Operator : SY/MD
Sample : P1822-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0786

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034889.D
Acq On : 28 Mar 2024 16:22
Operator : SY/MD
Sample : P1822-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0786

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------