

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034891.D
 Acq On : 28 Mar 2024 17:10
 Operator : SY/MD
 Sample : P1822-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	231328	242776	17.48%	2.289%
2	1.532	146	153	170	rVB	208641	246438	17.75%	2.323%
3	2.060	308	317	333	rVB	393708	566527	40.79%	5.340%
4	2.449	433	438	444	rBV6	1229	1833	0.13%	0.017%
5	2.642	496	498	503	rBV3	514	445	0.03%	0.004%
6	3.076	630	633	635	rBV3	435	198	0.01%	0.002%
7	3.185	664	667	669	rBV	284	185	0.01%	0.002%
8	3.230	677	681	683	rBV2	332	208	0.01%	0.002%
9	3.243	683	685	691	rVB	464	325	0.02%	0.003%
10	3.320	706	709	713	rBV2	478	406	0.03%	0.004%
11	3.449	747	749	750	rBV	384	181	0.01%	0.002%
12	3.487	760	761	762	rVB	236	46	0.00%	0.000%
13	3.500	762	765	766	rBV2	407	237	0.02%	0.002%
14	3.706	825	829	832	rBV3	479	427	0.03%	0.004%
15	3.790	847	855	890	rBV	84019	248480	17.89%	2.342%
16	4.249	983	998	1026	rBV2	210883	543426	39.13%	5.123%
17	4.516	1077	1081	1084	rBV2	454	386	0.03%	0.004%
18	4.690	1129	1135	1138	rBV2	637	837	0.06%	0.008%
19	4.818	1173	1175	1178	rBV	432	313	0.02%	0.003%
20	4.957	1201	1218	1252	rBV2	528695	1388763	100.00%	13.091%
21	5.378	1347	1349	1352	rBV	365	214	0.02%	0.002%
22	5.532	1385	1397	1428	rBV	415166	858533	61.82%	8.093%
23	5.789	1473	1477	1478	rBV3	576	377	0.03%	0.004%
24	5.831	1482	1490	1511	rVB2	11025	24785	1.78%	0.234%
25	5.944	1522	1525	1526	rBV2	651	390	0.03%	0.004%
26	5.989	1526	1539	1567	rVV	297629	624803	44.99%	5.890%
27	6.365	1652	1656	1660	rBV2	453	463	0.03%	0.004%
28	6.500	1697	1698	1702	rBV	277	174	0.01%	0.002%
29	6.635	1739	1740	1741	rBV	238	53	0.00%	0.000%
30	6.667	1748	1750	1753	rBV2	355	249	0.02%	0.002%
31	6.744	1769	1774	1776	rBV3	422	318	0.02%	0.003%
32	6.761	1776	1779	1784	rVB4	561	455	0.03%	0.004%
33	6.786	1784	1787	1789	rBV3	488	315	0.02%	0.003%
34	6.806	1791	1793	1797	rBV2	287	238	0.02%	0.002%
35	6.915	1816	1827	1856	rBV	148937	289663	20.86%	2.731%
36	7.243	1918	1929	1967	rBV	624971	1105605	79.61%	10.422%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034891.D
 Acq On : 28 Mar 2024 17:10
 Operator : SY/MD
 Sample : P1822-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	7.555	2017	2026	2048	rBV	103196	189460	13.64%	1.786%
38	7.908	2134	2136	2137	rBV	382	121	0.01%	0.001%
39	7.973	2153	2156	2158	rBV	271	217	0.02%	0.002%
40	8.027	2164	2173	2218	rBV2	268942	588538	42.38%	5.548%
41	8.783	2398	2408	2427	rBV	649095	1059491	76.29%	9.987%
42	9.188	2531	2534	2539	rBV2	753	708	0.05%	0.007%
43	9.297	2566	2568	2569	rBV2	360	114	0.01%	0.001%
44	9.339	2579	2581	2584	rBV	371	186	0.01%	0.002%
45	9.420	2602	2606	2608	rBV	356	327	0.02%	0.003%
46	9.484	2623	2626	2628	rBV2	355	202	0.01%	0.002%
47	9.603	2660	2663	2665	rBV2	479	296	0.02%	0.003%
48	9.706	2694	2695	2696	rBV2	232	82	0.01%	0.001%
49	10.034	2794	2797	2798	rBV	251	138	0.01%	0.001%
50	10.153	2822	2834	2857	rBV	402359	640107	46.09%	6.034%
51	10.580	2962	2967	2971	rBV2	385	435	0.03%	0.004%
52	10.963	3083	3086	3087	rBV2	451	281	0.02%	0.003%
53	11.085	3119	3124	3129	rBV	449	530	0.04%	0.005%
54	11.130	3135	3138	3142	rVB2	754	544	0.04%	0.005%
55	11.185	3143	3155	3185	rBV	641185	1006166	72.45%	9.485%
56	11.558	3259	3271	3298	rBV	617696	962968	69.34%	9.078%
57	12.786	3652	3653	3657	rBV	397	302	0.02%	0.003%
58	12.844	3666	3671	3680	rBV	9338	7915	0.57%	0.075%




Sum of corrected areas: 10608200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034891.D
Acq On : 28 Mar 2024 17:10
Operator : SY/MD
Sample : P1822-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

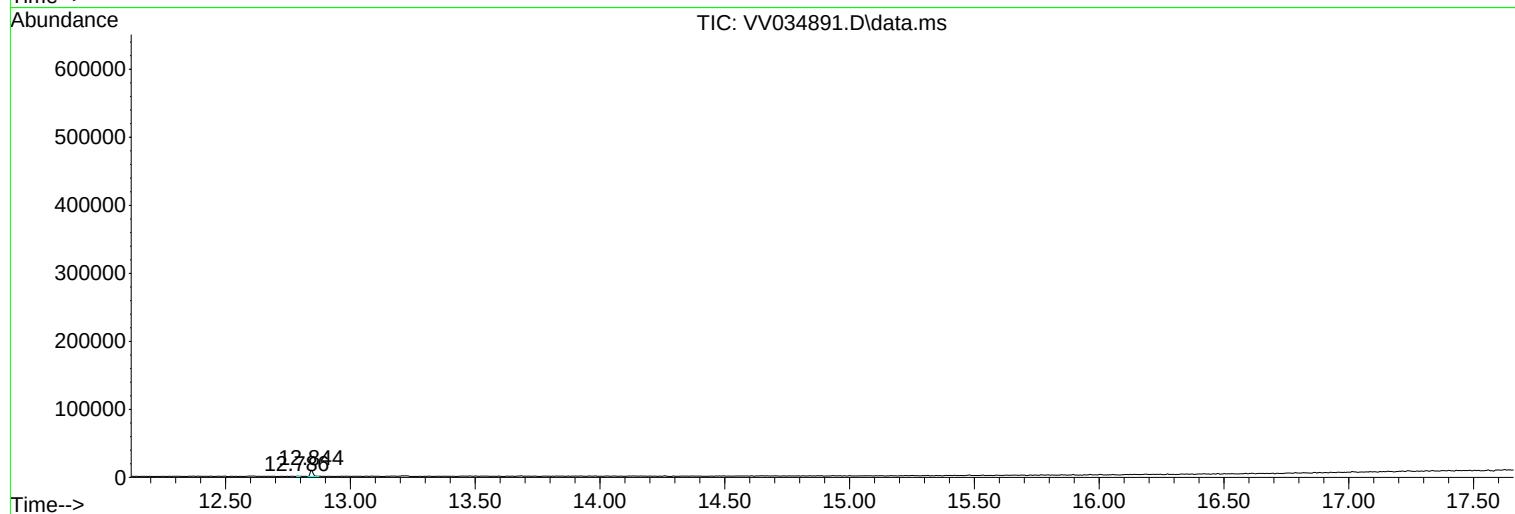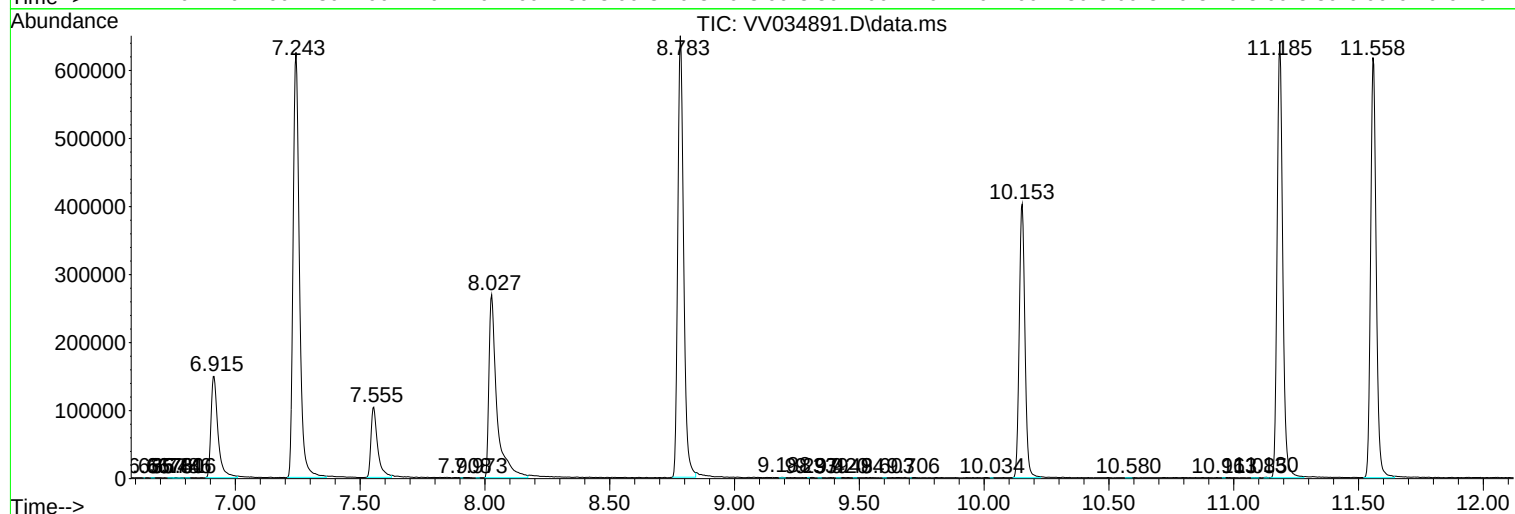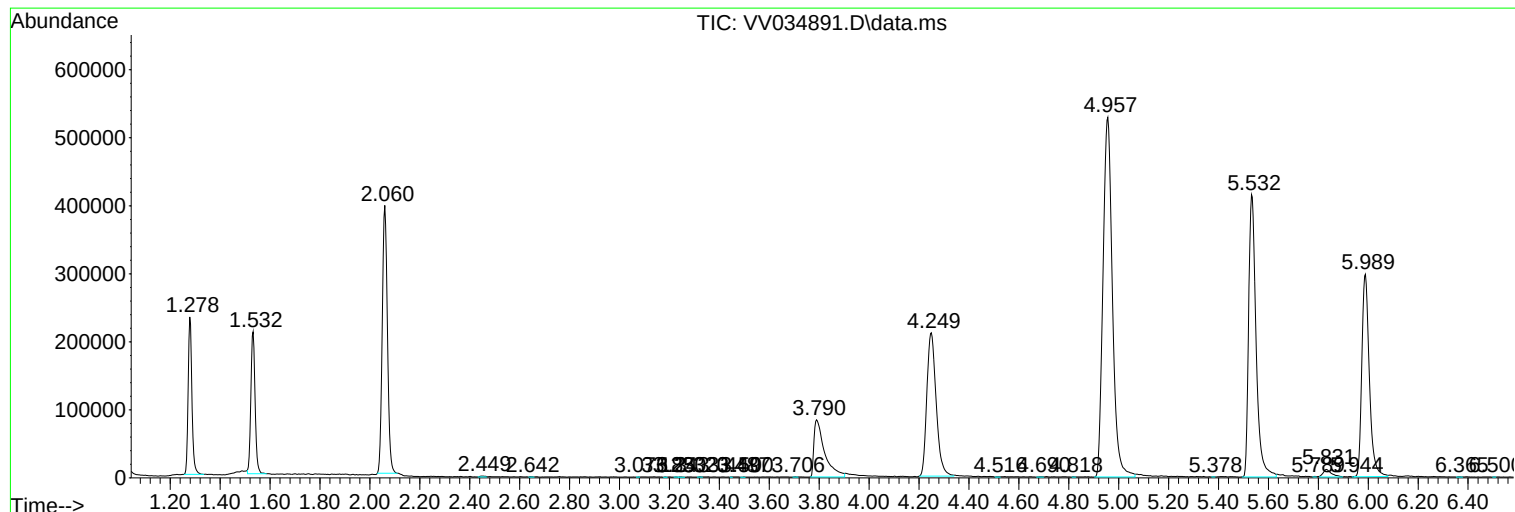

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034891.D
Acq On : 28 Mar 2024 17:10
Operator : SY/MD
Sample : P1822-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034891.D
Acq On : 28 Mar 2024 17:10
Operator : SY/MD
Sample : P1822-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
