

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034892.D
 Acq On : 28 Mar 2024 17:34
 Operator : SY/MD
 Sample : P1851-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	230917	244095	17.17%	2.294%
2	1.532	146	153	172	rVB	209294	249642	17.56%	2.346%
3	2.059	307	317	332	rBV	391129	566509	39.84%	5.324%
4	2.246	368	375	377	rBV2	1710	1779	0.13%	0.017%
5	2.416	426	428	429	rBV	527	241	0.02%	0.002%
6	2.526	459	462	464	rVB	306	187	0.01%	0.002%
7	2.542	464	467	469	rBV	316	215	0.02%	0.002%
8	2.770	535	538	539	rBV	306	203	0.01%	0.002%
9	3.043	619	623	625	rBV	376	267	0.02%	0.003%
10	3.059	625	628	631	rVV	587	400	0.03%	0.004%
11	3.088	635	637	642	rVB3	332	266	0.02%	0.002%
12	3.121	645	647	650	rVB2	422	233	0.02%	0.002%
13	3.178	662	665	668	rVB2	293	183	0.01%	0.002%
14	3.201	668	672	675	rBV2	319	243	0.02%	0.002%
15	3.217	675	677	682	rVB3	261	231	0.02%	0.002%
16	3.333	710	713	716	rVV2	338	221	0.02%	0.002%
17	3.510	763	768	773	rBV3	564	584	0.04%	0.005%
18	3.567	783	786	790	rBV2	291	284	0.02%	0.003%
19	3.664	814	816	822	rVB2	305	221	0.02%	0.002%
20	3.696	822	826	829	rBV3	305	273	0.02%	0.003%
21	3.789	847	855	885	rBV	89908	253834	17.85%	2.385%
22	4.249	983	998	1031	rBV	219654	563381	39.62%	5.294%
23	4.603	1104	1108	1110	rBV2	531	346	0.02%	0.003%
24	4.744	1151	1152	1158	rVB2	548	358	0.03%	0.003%
25	4.786	1163	1165	1169	rVB2	428	266	0.02%	0.002%
26	4.873	1187	1192	1196	rVB2	509	474	0.03%	0.004%
27	4.956	1201	1218	1255	rBV2	532579	1421951	100.00%	13.363%
28	5.284	1318	1320	1323	rBV2	473	201	0.01%	0.002%
29	5.532	1387	1397	1427	rBV	389348	816009	57.39%	7.668%
30	5.834	1482	1491	1508	rBV4	10586	22519	1.58%	0.212%
31	5.989	1526	1539	1570	rBV	303313	636888	44.79%	5.985%
32	6.243	1614	1618	1623	rBV4	648	593	0.04%	0.006%
33	6.333	1643	1646	1652	rBV3	533	573	0.04%	0.005%
34	6.429	1674	1676	1682	rVB3	459	363	0.03%	0.003%
35	6.458	1682	1685	1688	rBV3	351	313	0.02%	0.003%
36	6.526	1702	1706	1708	rVB2	341	253	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034892.D
 Acq On : 28 Mar 2024 17:34
 Operator : SY/MD
 Sample : P1851-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.564	1713	1718	1719	rBV	269	195	0.01%	0.002%
38	6.619	1732	1735	1739	rBV	461	347	0.02%	0.003%
39	6.667	1748	1750	1754	rVB2	474	288	0.02%	0.003%
40	6.686	1754	1756	1758	rBV2	444	237	0.02%	0.002%
41	6.763	1769	1780	1783	rVB4	610	842	0.06%	0.008%
42	6.786	1783	1787	1789	rBV3	281	229	0.02%	0.002%
43	6.854	1806	1808	1813	rBV2	247	205	0.01%	0.002%
44	6.915	1816	1827	1854	rBV	157658	304198	21.39%	2.859%
45	7.162	1898	1904	1906	rBV3	517	617	0.04%	0.006%
46	7.243	1918	1929	1966	rBV	636289	1120831	78.82%	10.533%
47	7.554	2017	2026	2047	rBV	107965	196877	13.85%	1.850%
48	7.828	2109	2111	2117	rVB3	589	489	0.03%	0.005%
49	7.908	2132	2136	2137	rVB2	469	292	0.02%	0.003%
50	7.921	2137	2140	2144	rBV4	544	568	0.04%	0.005%
51	7.976	2155	2157	2160	rVB2	397	236	0.02%	0.002%
52	7.995	2160	2163	2164	rBV2	378	203	0.01%	0.002%
53	8.027	2164	2173	2211	rBV2	277327	603420	42.44%	5.671%
54	8.461	2305	2308	2313	rBV4	729	479	0.03%	0.005%
55	8.484	2313	2315	2319	rVB3	611	264	0.02%	0.002%
56	8.545	2331	2334	2339	rBV2	690	555	0.04%	0.005%
57	8.599	2349	2351	2354	rBV2	438	269	0.02%	0.003%
58	8.738	2392	2394	2396	rBV2	490	248	0.02%	0.002%
59	8.783	2397	2408	2436	rBV	612066	1016826	71.51%	9.556%
60	9.021	2480	2482	2484	rBV2	409	196	0.01%	0.002%
61	9.033	2484	2486	2490	rVB2	978	526	0.04%	0.005%
62	9.059	2490	2494	2495	rBV2	679	437	0.03%	0.004%
63	9.088	2500	2503	2505	rBV2	887	511	0.04%	0.005%
64	9.114	2509	2511	2515	rVB3	521	308	0.02%	0.003%
65	9.149	2520	2522	2525	rBV3	417	222	0.02%	0.002%
66	9.178	2529	2531	2533	rBV	521	298	0.02%	0.003%
67	9.207	2538	2540	2543	rBV2	557	307	0.02%	0.003%
68	9.339	2576	2581	2583	rBV	496	476	0.03%	0.004%
69	9.416	2601	2605	2607	rBV2	368	242	0.02%	0.002%
70	9.448	2612	2615	2618	rBV	250	212	0.01%	0.002%
71	9.542	2641	2644	2645	rBV	438	237	0.02%	0.002%
72	9.583	2652	2657	2662	rBV2	656	656	0.05%	0.006%
73	9.612	2662	2666	2667	rBV	425	275	0.02%	0.003%
74	9.728	2700	2702	2710	rVB2	243	189	0.01%	0.002%
75	9.770	2710	2715	2716	rBV	410	330	0.02%	0.003%
76	9.960	2772	2774	2781	rVB3	430	352	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
 Data File : VV034892.D
 Acq On : 28 Mar 2024 17:34
 Operator : SY/MD
 Sample : P1851-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.995	2781	2785	2788	rVB4	464	400	0.03%	0.004%
78	10.059	2802	2805	2807	rBV	368	230	0.02%	0.002%
79	10.152	2819	2834	2860	rBV	418464	672600	47.30%	6.321%
80	10.310	2881	2883	2886	rBV2	334	199	0.01%	0.002%
81	10.484	2934	2937	2940	rBV2	333	258	0.02%	0.002%
82	10.525	2945	2950	2953	rBV3	584	569	0.04%	0.005%
83	10.615	2974	2978	2981	rBV3	361	251	0.02%	0.002%
84	10.847	3047	3050	3053	rBV3	537	393	0.03%	0.004%
85	10.869	3053	3057	3062	rVB3	314	326	0.02%	0.003%
86	10.898	3062	3066	3067	rBV3	355	232	0.02%	0.002%
87	11.185	3144	3155	3180	rBV	600056	950349	66.83%	8.931%
88	11.558	3260	3271	3294	rBV	614005	971958	68.35%	9.134%
89	11.860	3361	3365	3367	rBV2	807	482	0.03%	0.005%
90	11.898	3373	3377	3380	rBV3	541	476	0.03%	0.004%
91	11.972	3398	3400	3409	rVB2	484	530	0.04%	0.005%
92	12.008	3409	3411	3414	rBV2	339	232	0.02%	0.002%
93	12.066	3427	3429	3434	rVB3	667	497	0.03%	0.005%
94	12.509	3565	3567	3570	rBV2	443	258	0.02%	0.002%
95	12.557	3578	3582	3585	rBV3	614	486	0.03%	0.005%
96	12.985	3712	3715	3718	rBV	419	293	0.02%	0.003%
97	13.037	3727	3731	3734	rVB2	356	278	0.02%	0.003%
98	13.249	3795	3797	3799	rBV	371	207	0.01%	0.002%
99	13.358	3829	3831	3834	rBV	423	310	0.02%	0.003%
100	13.638	3916	3918	3919	rBV	512	194	0.01%	0.002%




Sum of corrected areas: 10641096

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034892.D
Acq On : 28 Mar 2024 17:34
Operator : SY/MD
Sample : P1851-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

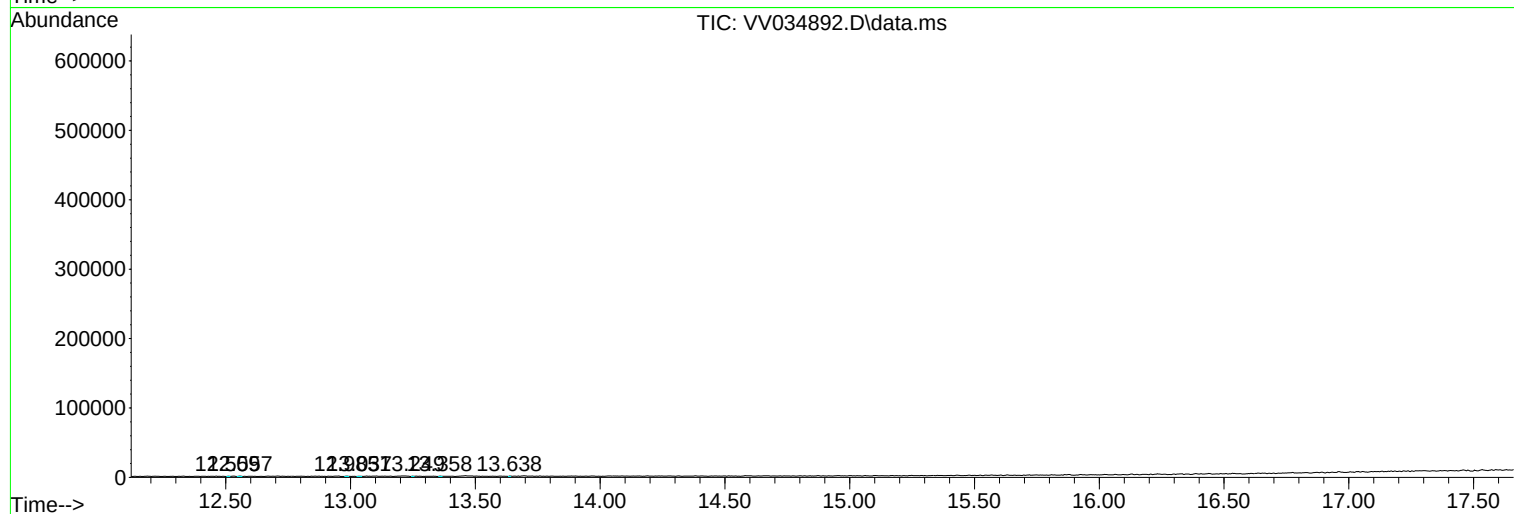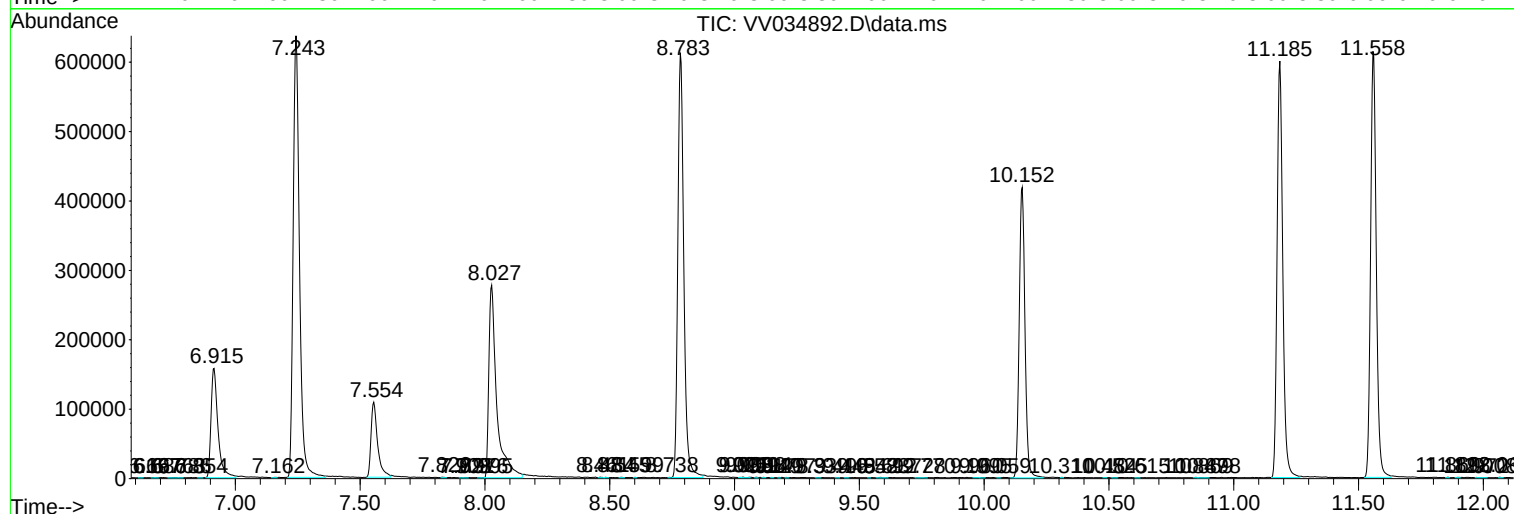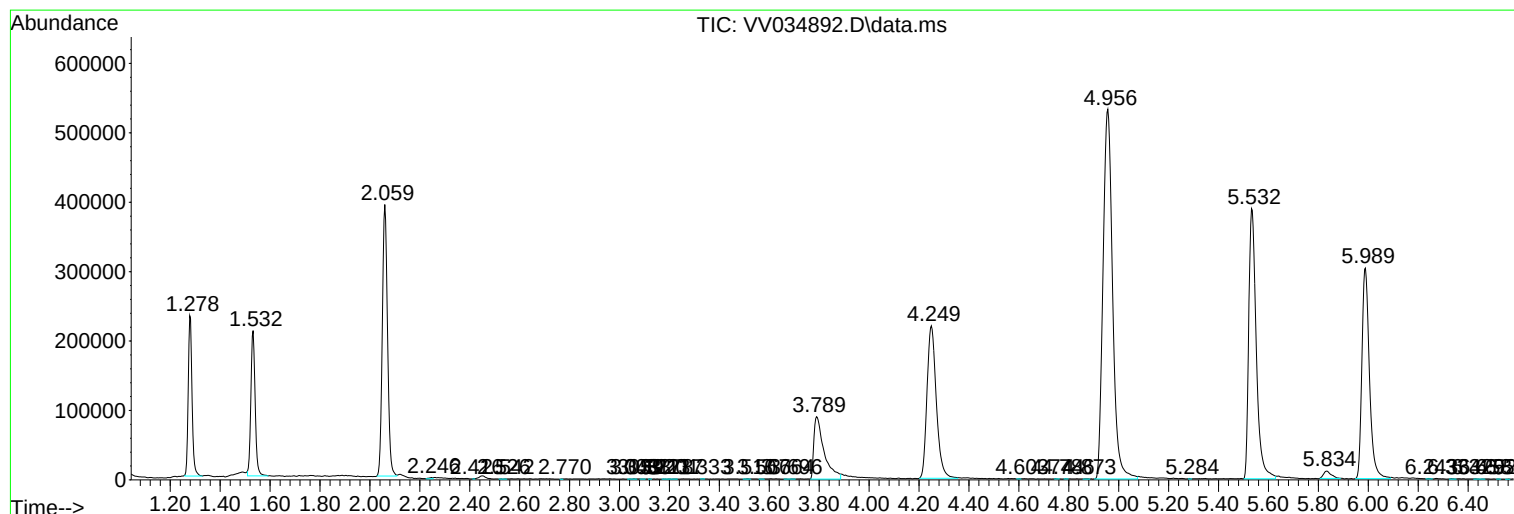

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034892.D
Acq On : 28 Mar 2024 17:34
Operator : SY/MD
Sample : P1851-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034892.D
Acq On : 28 Mar 2024 17:34
Operator : SY/MD
Sample : P1851-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------