
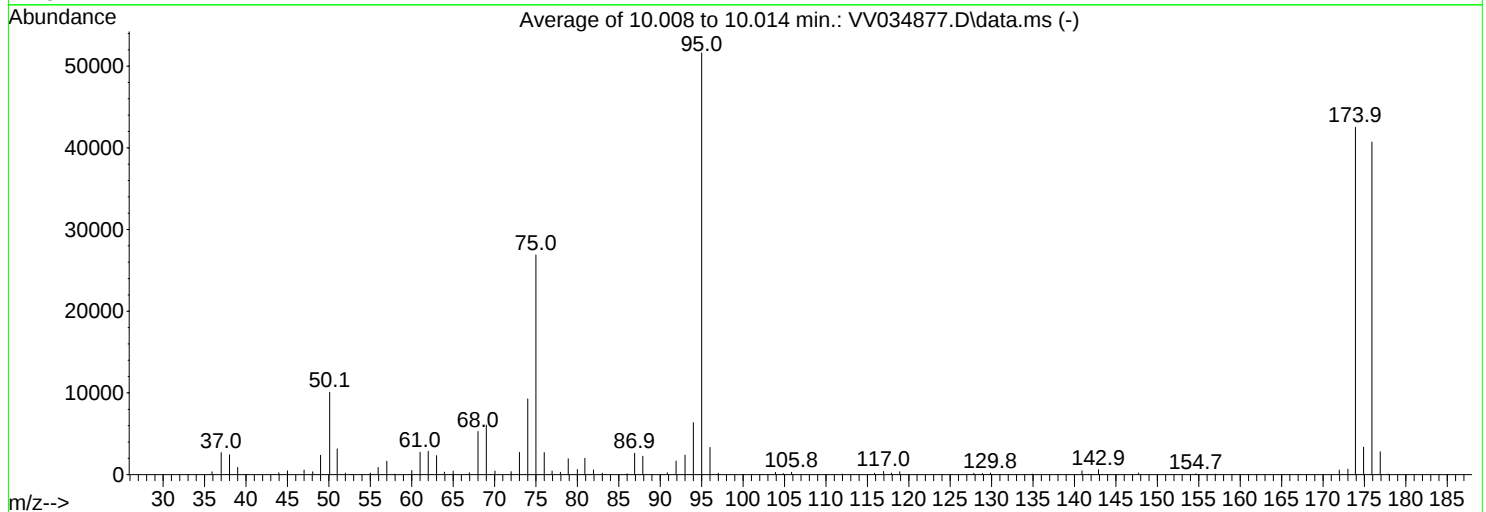


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032824\
Data File : VV034877.D
Acq On : 28 Mar 2024 11:04
Operator : SY/MD
Sample : BFB277
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB277

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Fri Mar 29 00:23:40 2024

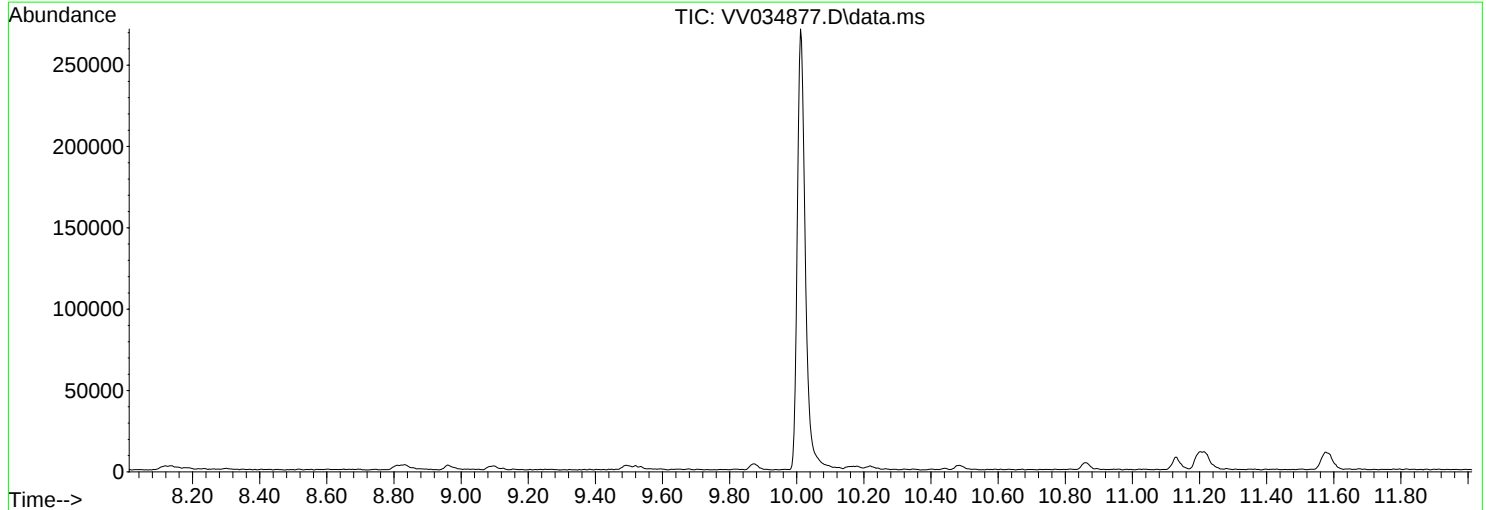

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10095	PASS
75	95	30	80	52.1	26885	PASS
95	95	100	100	100.0	51629	PASS
96	95	5	9	6.5	3334	PASS
173	174	0.00	2	1.6	660	PASS
174	95	50	120	82.4	42523	PASS
175	174	5	9	7.9	3367	PASS
176	174	95	105	95.8	40723	PASS
177	176	5	10	6.9	2795	PASS

m/z	Abundance
35.80	103.0
39.90	920.0
43.90	430.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
36.00	471.0
37.00	2636.0
38.00	2418.0
39.00	903.0
40.00	976.0
44.00	683.0
45.00	443.0
47.00	523.0
48.10	373.0
49.00	2340.0
50.10	9833.0
51.00	3056.0
52.00	216.0
52.80	112.0
55.00	171.0
55.90	832.0
57.00	1599.0
58.00	112.0
60.00	446.0
61.00	2637.0
62.00	2861.0
63.00	2330.0
63.90	321.0
65.00	344.0
66.90	260.0
68.00	5113.0
69.00	5976.0
70.10	473.0
72.00	316.0
73.00	2724.0
74.00	9124.0
75.00	25720.0
76.00	2511.0
76.90	479.0
78.00	297.0
78.90	1834.0
80.00	616.0
80.90	1875.0
82.00	587.0
83.00	185.0
86.00	113.0
86.90	2625.0
87.90	2226.0
90.80	241.0
91.90	1639.0
93.00	2378.0
94.00	6048.0
95.00	49416.0
96.00	3400.0
97.00	160.0
103.90	270.0
104.90	143.0
105.90	317.0
115.80	167.0
116.90	374.0
117.90	165.0
118.90	340.0
127.80	201.0
128.90	113.0
129.80	170.0
134.90	104.0
140.90	422.0
142.90	542.0
147.70	204.0
154.70	118.0
157.00	108.0
172.00	552.0
173.00	642.0
173.90	39440.0
174.90	3176.0
175.90	37656.0
176.90	2839.0
177.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
36.00	477.0
37.00	2806.0
38.00	2474.0
39.00	874.0
40.00	961.0
44.00	660.0
45.00	494.0
47.00	586.0
48.10	372.0
49.00	2455.0
50.10	10498.0
51.00	3259.0
52.00	197.0
55.00	200.0
55.90	901.0
57.00	1701.0
60.00	497.0
61.00	2820.0
62.00	2998.0
63.00	2422.0
64.00	339.0
65.00	437.0
66.90	227.0
68.00	5428.0
69.00	6305.0
70.10	460.0
72.00	397.0
73.00	2835.0
74.00	9599.0
75.00	27920.0
76.00	2829.0
77.00	444.0
78.00	289.0
78.90	1994.0
80.00	640.0
80.90	2044.0
82.00	609.0
83.00	194.0
86.00	130.0
86.90	2750.0
87.90	2329.0
90.90	240.0
91.90	1756.0
93.00	2493.0
94.00	6594.0
95.00	53528.0
96.00	3412.0
97.00	183.0
103.90	294.0
104.80	145.0
105.80	300.0
112.00	122.0
115.90	188.0
116.90	397.0
117.90	203.0
118.90	369.0
127.80	169.0
128.90	138.0
129.90	194.0
134.90	116.0
140.90	491.0
142.90	629.0
147.80	185.0
154.60	118.0
157.00	114.0
171.90	553.0
173.00	705.0
173.90	44024.0
174.90	3459.0
175.90	42216.0
176.90	2916.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
35.90	443.0
37.00	2663.0
38.00	2379.0
39.00	863.0
40.00	925.0
44.00	655.0
45.00	506.0
47.00	604.0
47.90	323.0
49.00	2294.0
50.10	9953.0
51.00	3118.0
52.00	189.0
55.00	223.0
56.00	888.0
57.00	1610.0
57.90	112.0
60.00	564.0
61.00	2796.0
62.00	2714.0
63.00	2266.0
64.00	310.0
65.00	494.0
67.00	205.0
68.00	5312.0
69.00	5928.0
70.00	409.0
72.00	419.0
73.00	2590.0
74.00	9066.0
75.00	27016.0
76.00	2774.0
77.00	404.0
77.80	273.0
78.90	2019.0
80.00	607.0
80.90	2056.0
81.90	524.0
83.00	168.0
86.00	127.0
86.90	2479.0
87.90	2218.0
90.90	230.0
91.90	1579.0
93.00	2295.0
94.00	6480.0
95.00	51944.0
96.00	3190.0
97.00	160.0
103.90	284.0
104.80	111.0
105.80	256.0
112.00	106.0
115.90	187.0
117.00	404.0
117.90	215.0
118.90	326.0
127.90	192.0
128.90	142.0
129.90	203.0
140.90	523.0
141.70	106.0
142.90	661.0
147.80	181.0
154.60	119.0
171.90	589.0
173.00	632.0
173.90	44104.0
174.90	3467.0
175.90	42296.0
176.90	2631.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277