




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025294.D
 Acq On : 29 Mar 2022 15:40
 Operator : SY/MD
 Sample : N2165-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/01/2022
 Supervised By :Mahesh Dadoda 04/01/2022

Quant Time: Mar 30 02:06:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 30 02:04:47 2022
 Response via : Initial Calibration

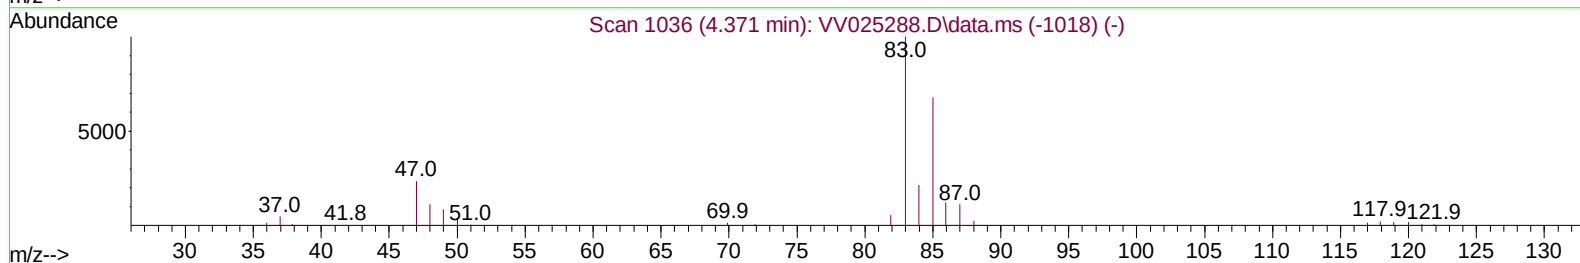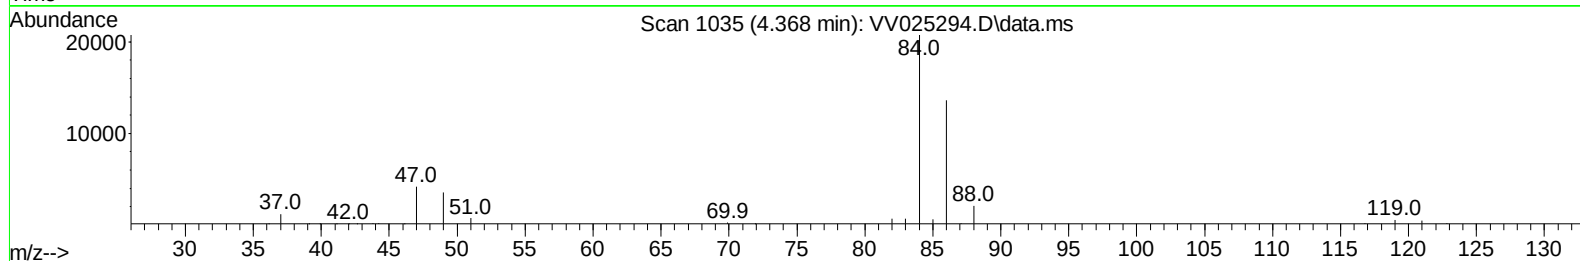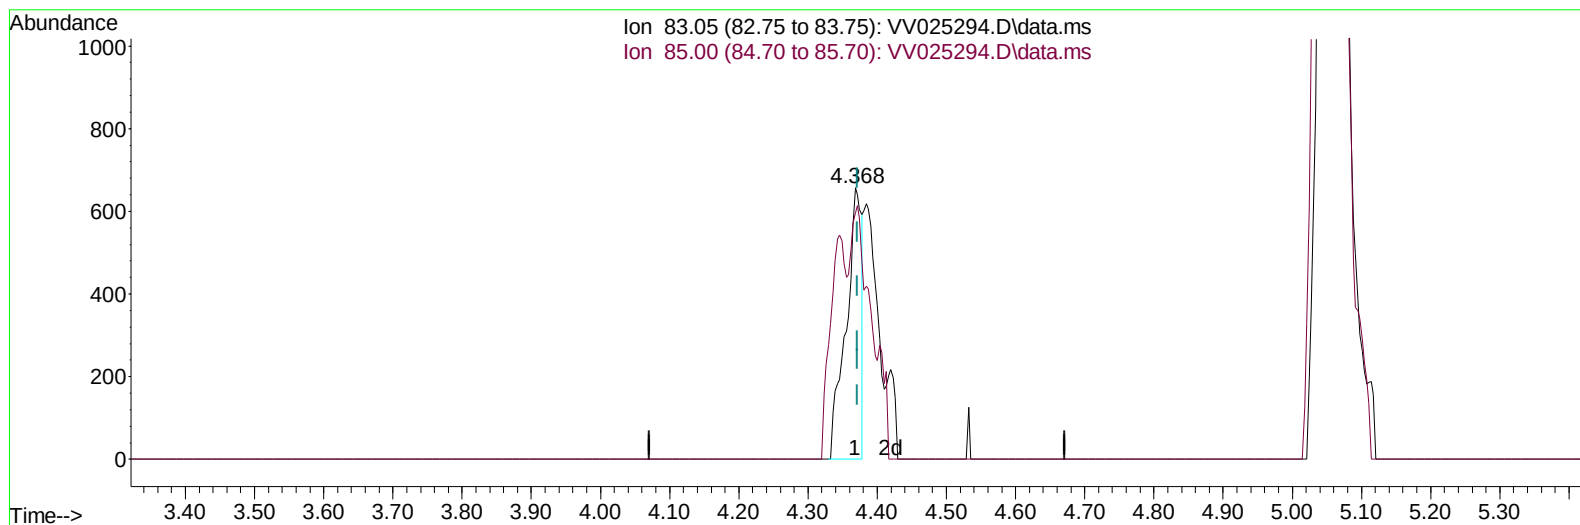

TIC: VV025294.D\data.ms

(25) Chloroform (T)

4.368min (-0.003) 0.05 ug/L

response 1033

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	90.87#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025294.D
 Acq On : 29 Mar 2022 15:40
 Operator : SY/MD
 Sample : N2165-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/01/2022
 Supervised By :Mahesh Dadoda 04/01/2022

Quant Time: Mar 30 02:06:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 30 02:04:47 2022
 Response via : Initial Calibration

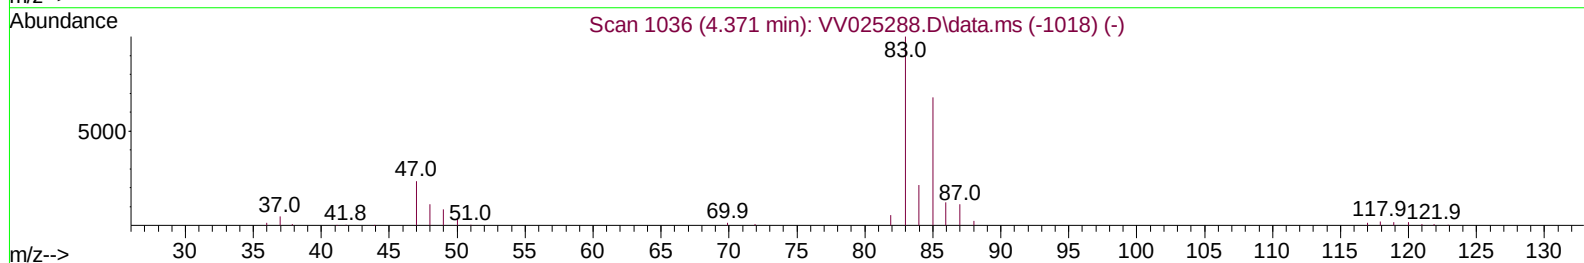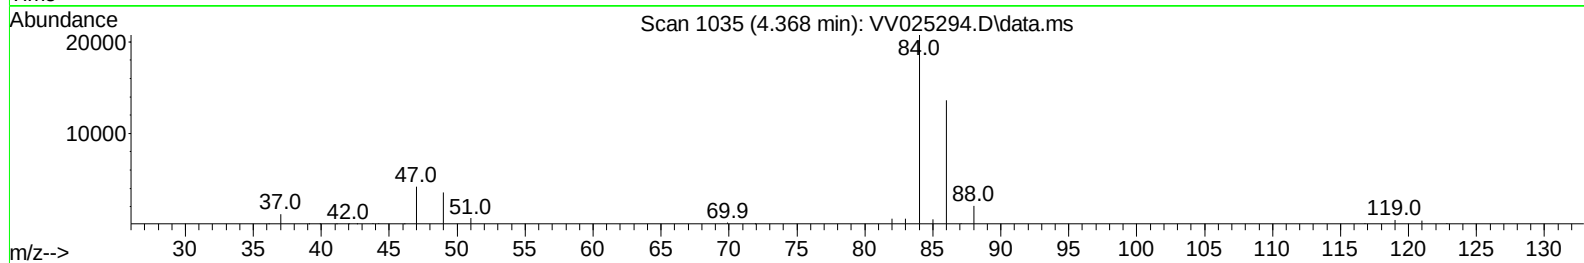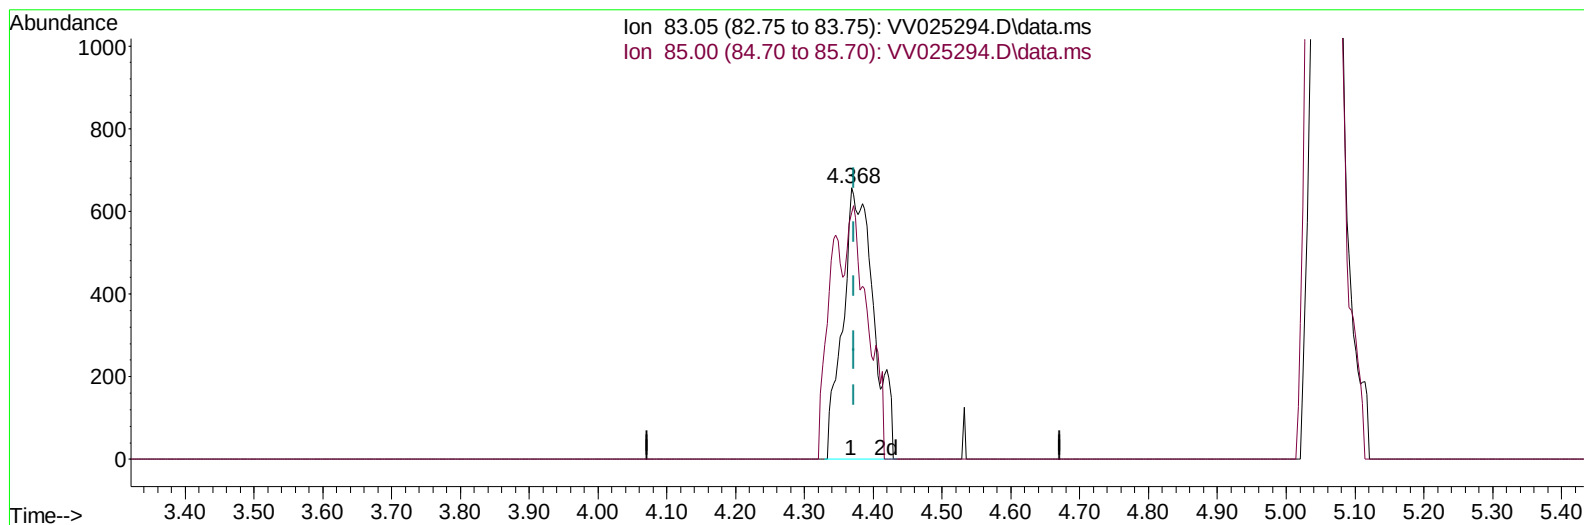

TIC: VV025294.D\data.ms

(25) Chloroform (T)

4.368min (-0.003) 0.10 ug/L m

response 2053

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	63.80	90.87#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025294.D
 Acq On : 29 Mar 2022 15:40
 Operator : SY/MD
 Sample : N2165-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R0

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:06:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 30 02:04:47 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 04/01/2022
 Supervised By : Mahesh Dadoda 04/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	147486	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	142669	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62107	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	70356	5.107	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	102.200%		
7) Chloroethane-d5	1.571	69	57390	4.963	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	99.200%		
11) 1,1-Dichloroethene-d2	2.111	63	99194	3.324	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	66.400%		
20) 2-Butanone-d5	3.892	46	66509	48.466	ug/L	-0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	96.940%		
24) Chloroform-d	4.352	84	88721	4.935	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	98.600%		
26) 1,2-Dichloroethane-d4	5.034	65	40357	5.078	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	101.600%		
32) Benzene-d6	5.050	84	178030	4.932	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	98.600%		
36) 1,2-Dichloropropane-d6	6.069	67	49849	4.928	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	98.600%		
41) Toluene-d8	7.317	98	154180	4.657	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	93.200%		
43) trans-1,3-Dichloroprop...	7.625	79	14929	4.524	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	90.400%		
46) 2-Hexanone-d5	8.088	63	50051	41.995	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	84.000%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31553	4.678	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	93.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152	51560	5.169	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	103.400%		
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	4968	0.426	ug/L	90
25) Chloroform	4.368	83	2053m	0.104	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025294.D
Acq On : 29 Mar 2022 15:40
Operator : SY/MD
Sample : N2165-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6R0

Manual IntegrationsAPPROVED

Quant Time: Mar 30 02:06:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 30 02:04:47 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/01/2022
Supervised By :Mahesh Dadoda 04/01/2022

