

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032922\
 Data File : VW025289.D
 Acq On : 29 Mar 2022 13:11
 Operator : SY/MD
 Sample : VW0329WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK329

Quant Time: Mar 30 02:05:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 30 02:04:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	156450	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	151974	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	63175	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	69282	4.741	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.800%
7) Chloroethane-d5	1.568	69	56742	4.626	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.600%
11) 1,1-Dichloroethene-d2	2.108	63	98914	3.125	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.400%
20) 2-Butanone-d5	3.902	46	59252	40.703	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.400%
24) Chloroform-d	4.346	84	84508	4.431	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
26) 1,2-Dichloroethane-d4	5.031	65	38188	4.530	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
32) Benzene-d6	5.047	84	174189	4.531	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.066	67	48010	4.456	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.200%
41) Toluene-d8	7.310	98	151137	4.286	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%
43) trans-1,3-Dichloroprop...	7.622	79	14028	3.991	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.088	63	47810	37.659	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.320%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29572	4.116	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	49758	4.904	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%
Target Compounds					Qvalue	
25) Chloroform	4.368	83	1910	0.091	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025289.D
Acq On : 29 Mar 2022 13:11
Operator : SY/MD
Sample : VV0329WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK329

Quant Time: Mar 30 02:05:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 30 02:04:47 2022
Response via : Initial Calibration

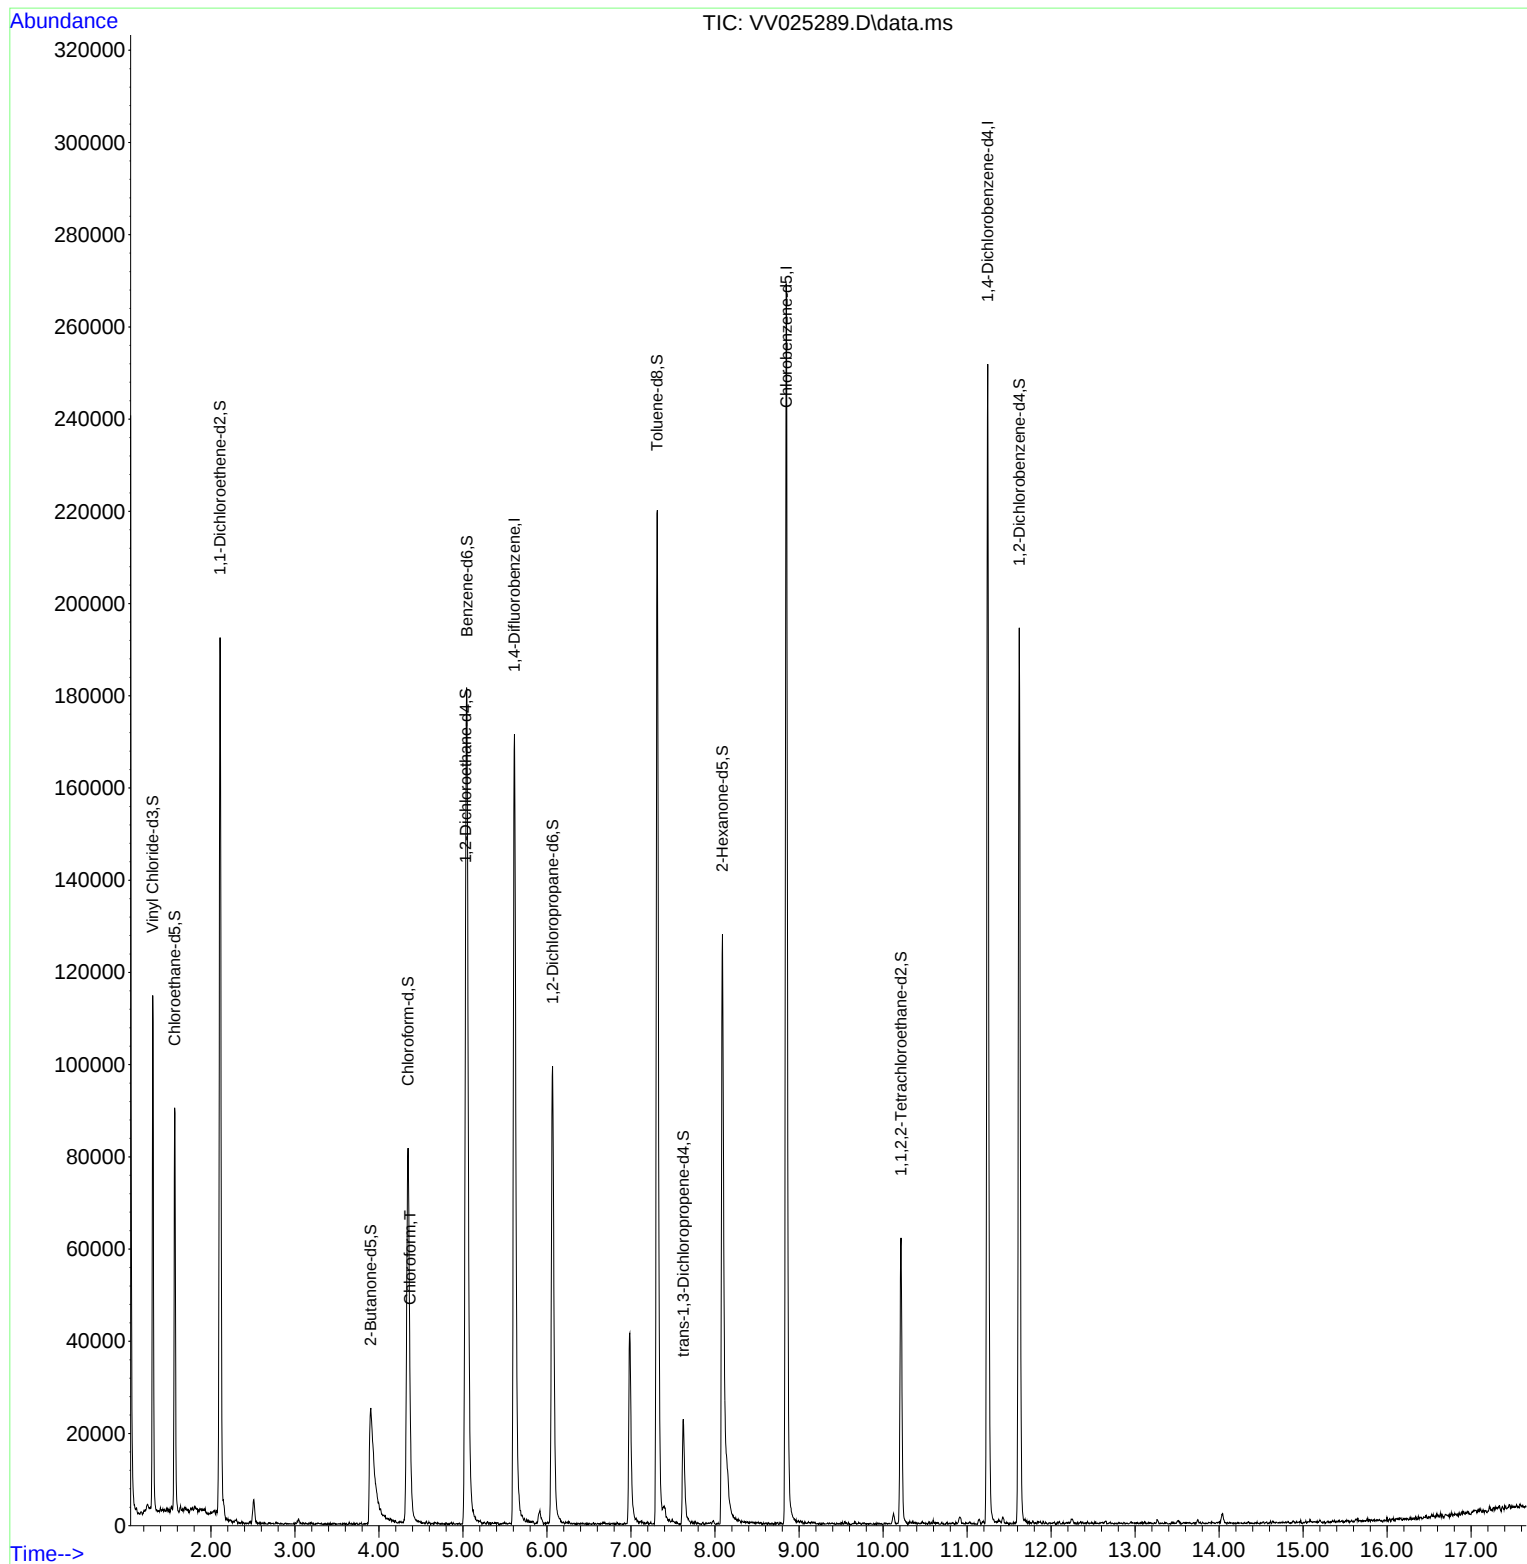

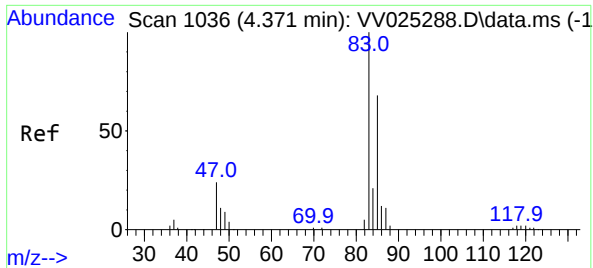

#25
Chloroform
Concen: 0.091 ug/L
RT: 4.368 min Scan# 10
Delta R.T. -0.003 min
Lab File: VV025289.D
Acq: 29 Mar 2022 13:11

Instrument :
MSVOA_V
ClientSampleId :
VBLK329

Tgt Ion: 83 Resp: 1910
Ion Ratio Lower Upper
83 100
85 78.6 44.7 82.9

