

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032922\
 Data File : VW025290.D
 Acq On : 29 Mar 2022 13:44
 Operator : SY/MD
 Sample : N2101-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Mar 30 02:05:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 30 02:04:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	197121	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	189340	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	82622	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	81831	4.444	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.800%
7) Chloroethane-d5	1.568	69	63135	4.085	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.800%
11) 1,1-Dichloroethene-d2	2.108	63	119861	3.005	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.200%
20) 2-Butanone-d5	3.905	46	69251	37.757	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.520%
24) Chloroform-d	4.346	84	96309	4.008	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.200%
26) 1,2-Dichloroethane-d4	5.031	65	42812	4.031	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.600%
32) Benzene-d6	5.047	84	204134	4.262	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.200%
36) 1,2-Dichloropropane-d6	6.066	67	56332	4.196	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.000%
41) Toluene-d8	7.313	98	173647	3.952	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
43) trans-1,3-Dichloroprop...	7.622	79	16690	3.811	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.200%
46) 2-Hexanone-d5	8.088	63	55697	35.213	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.420%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	34744	3.882	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	57486	4.332	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.600%
Target Compounds						
					Qvalue	
25) Chloroform	4.371	83	2203	0.083	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025290.D
Acq On : 29 Mar 2022 13:44
Operator : SY/MD
Sample : N2101-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Mar 30 02:05:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 30 02:04:47 2022
Response via : Initial Calibration

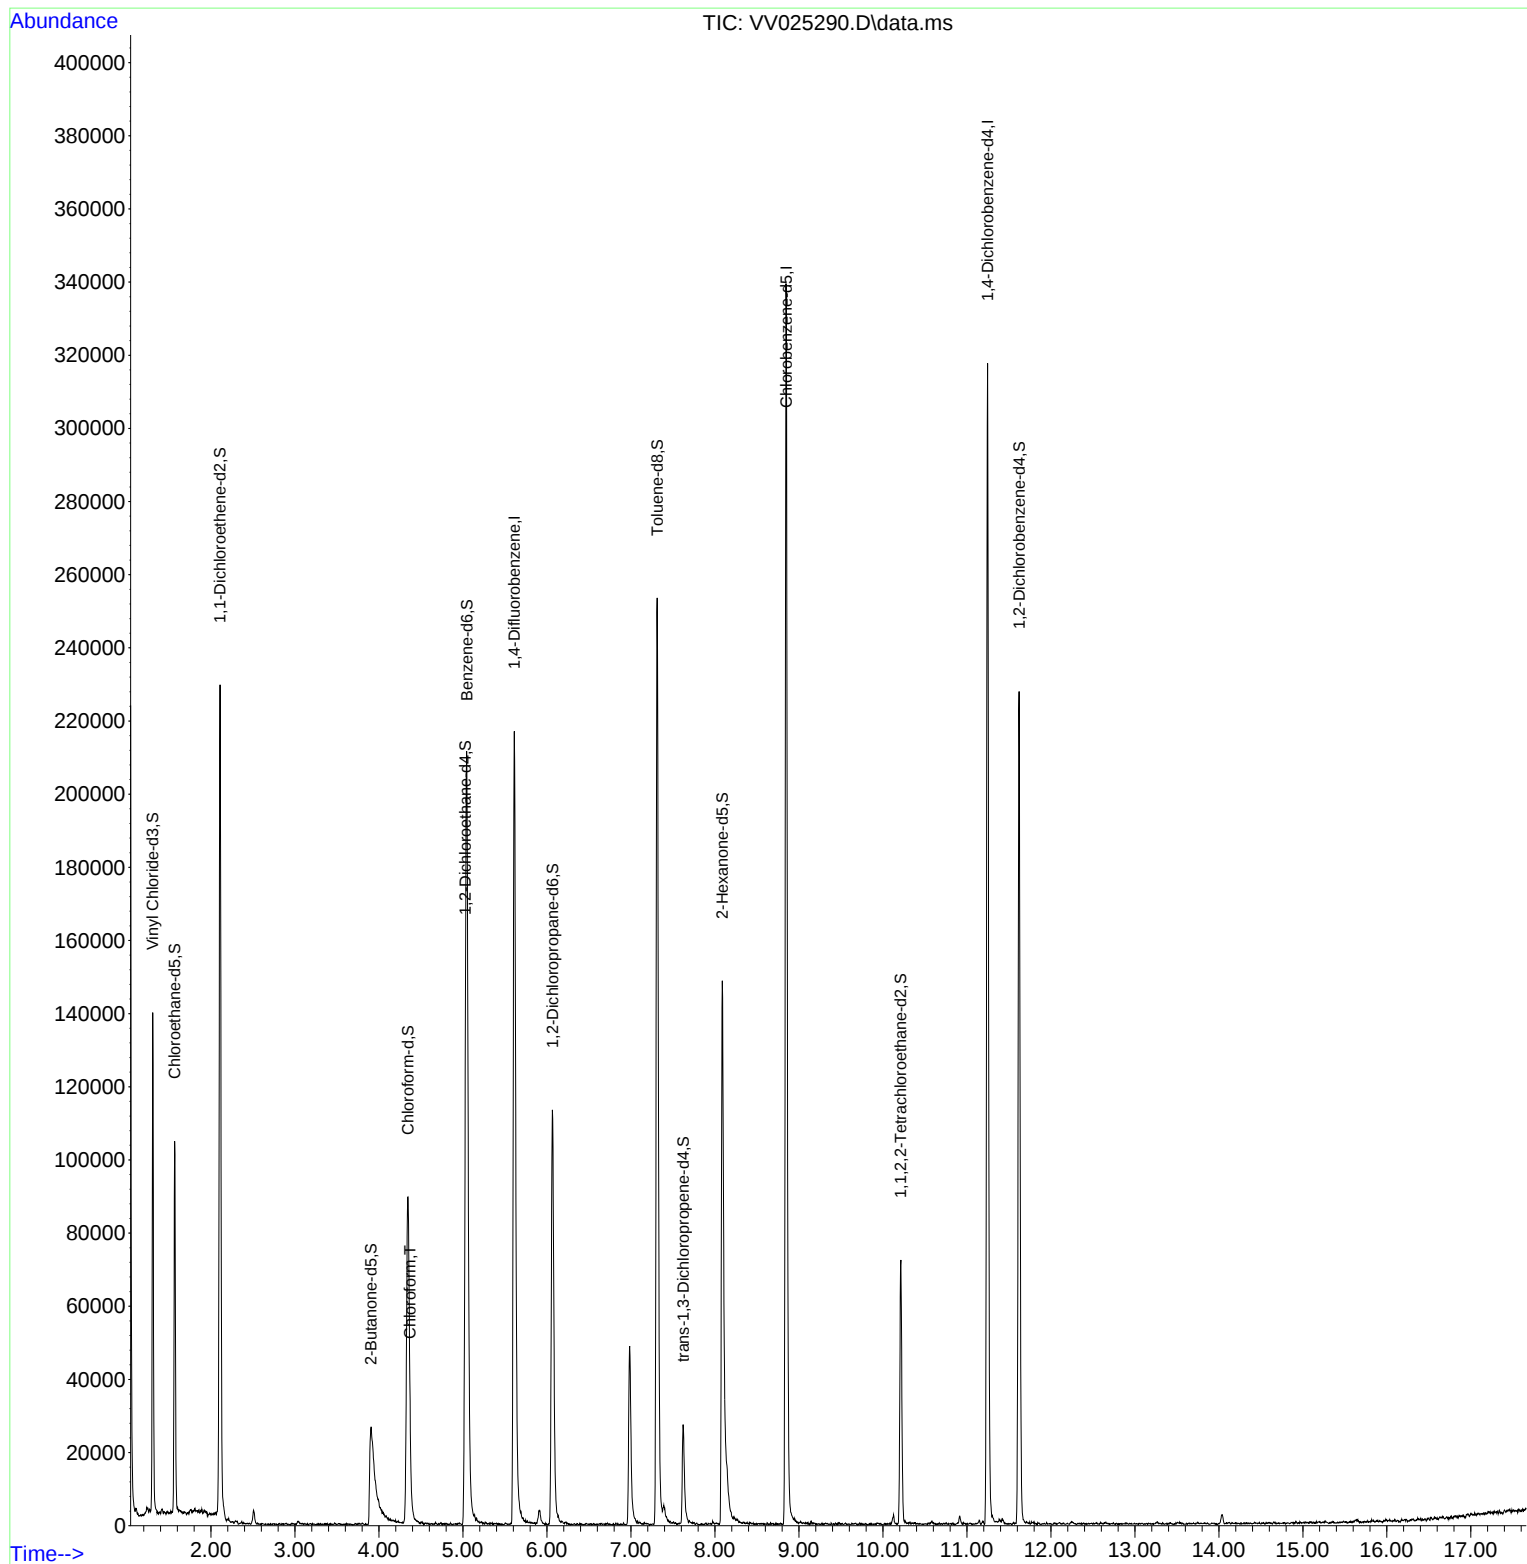

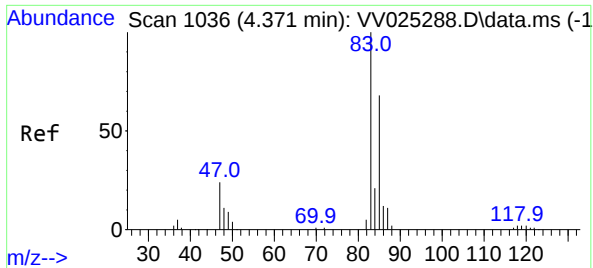

#25
 Chloroform
 Concen: 0.083 ug/L
 RT: 4.371 min Scan# 10
 Delta R.T. 0.000 min
 Lab File: VV025290.D
 Acq: 29 Mar 2022 13:44

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 83	Resp:	2203
Ion	Ratio	Lower Upper
83	100	
85	79.0	44.7 82.9

