

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032922\
 Data File : VW025293.D
 Acq On : 29 Mar 2022 15:17
 Operator : SY/MD
 Sample : N2165-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q8

Quant Time: Mar 30 02:06:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 30 02:04:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	148481	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	142662	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60857	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	73579	5.305	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.200%
7) Chloroethane-d5	1.571	69	58675	5.041	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.800%
11) 1,1-Dichloroethene-d2	2.111	63	106959	3.560	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.200%
20) 2-Butanone-d5	3.908	46	62970	45.579	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.160%
24) Chloroform-d	4.349	84	89793	4.961	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
26) 1,2-Dichloroethane-d4	5.034	65	39749	4.968	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.053	84	181222	5.021	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
36) 1,2-Dichloropropane-d6	6.069	67	50310	4.974	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.400%
41) Toluene-d8	7.317	98	156150	4.717	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
43) trans-1,3-Dichloroprop...	7.625	79	15414	4.671	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.400%
46) 2-Hexanone-d5	8.092	63	50676	42.522	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.040%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29882	4.431	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	51338	5.252	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	6766	0.576	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025293.D
Acq On : 29 Mar 2022 15:17
Operator : SY/MD
Sample : N2165-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q8


Quant Time: Mar 30 02:06:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 30 02:04:47 2022
Response via : Initial Calibration

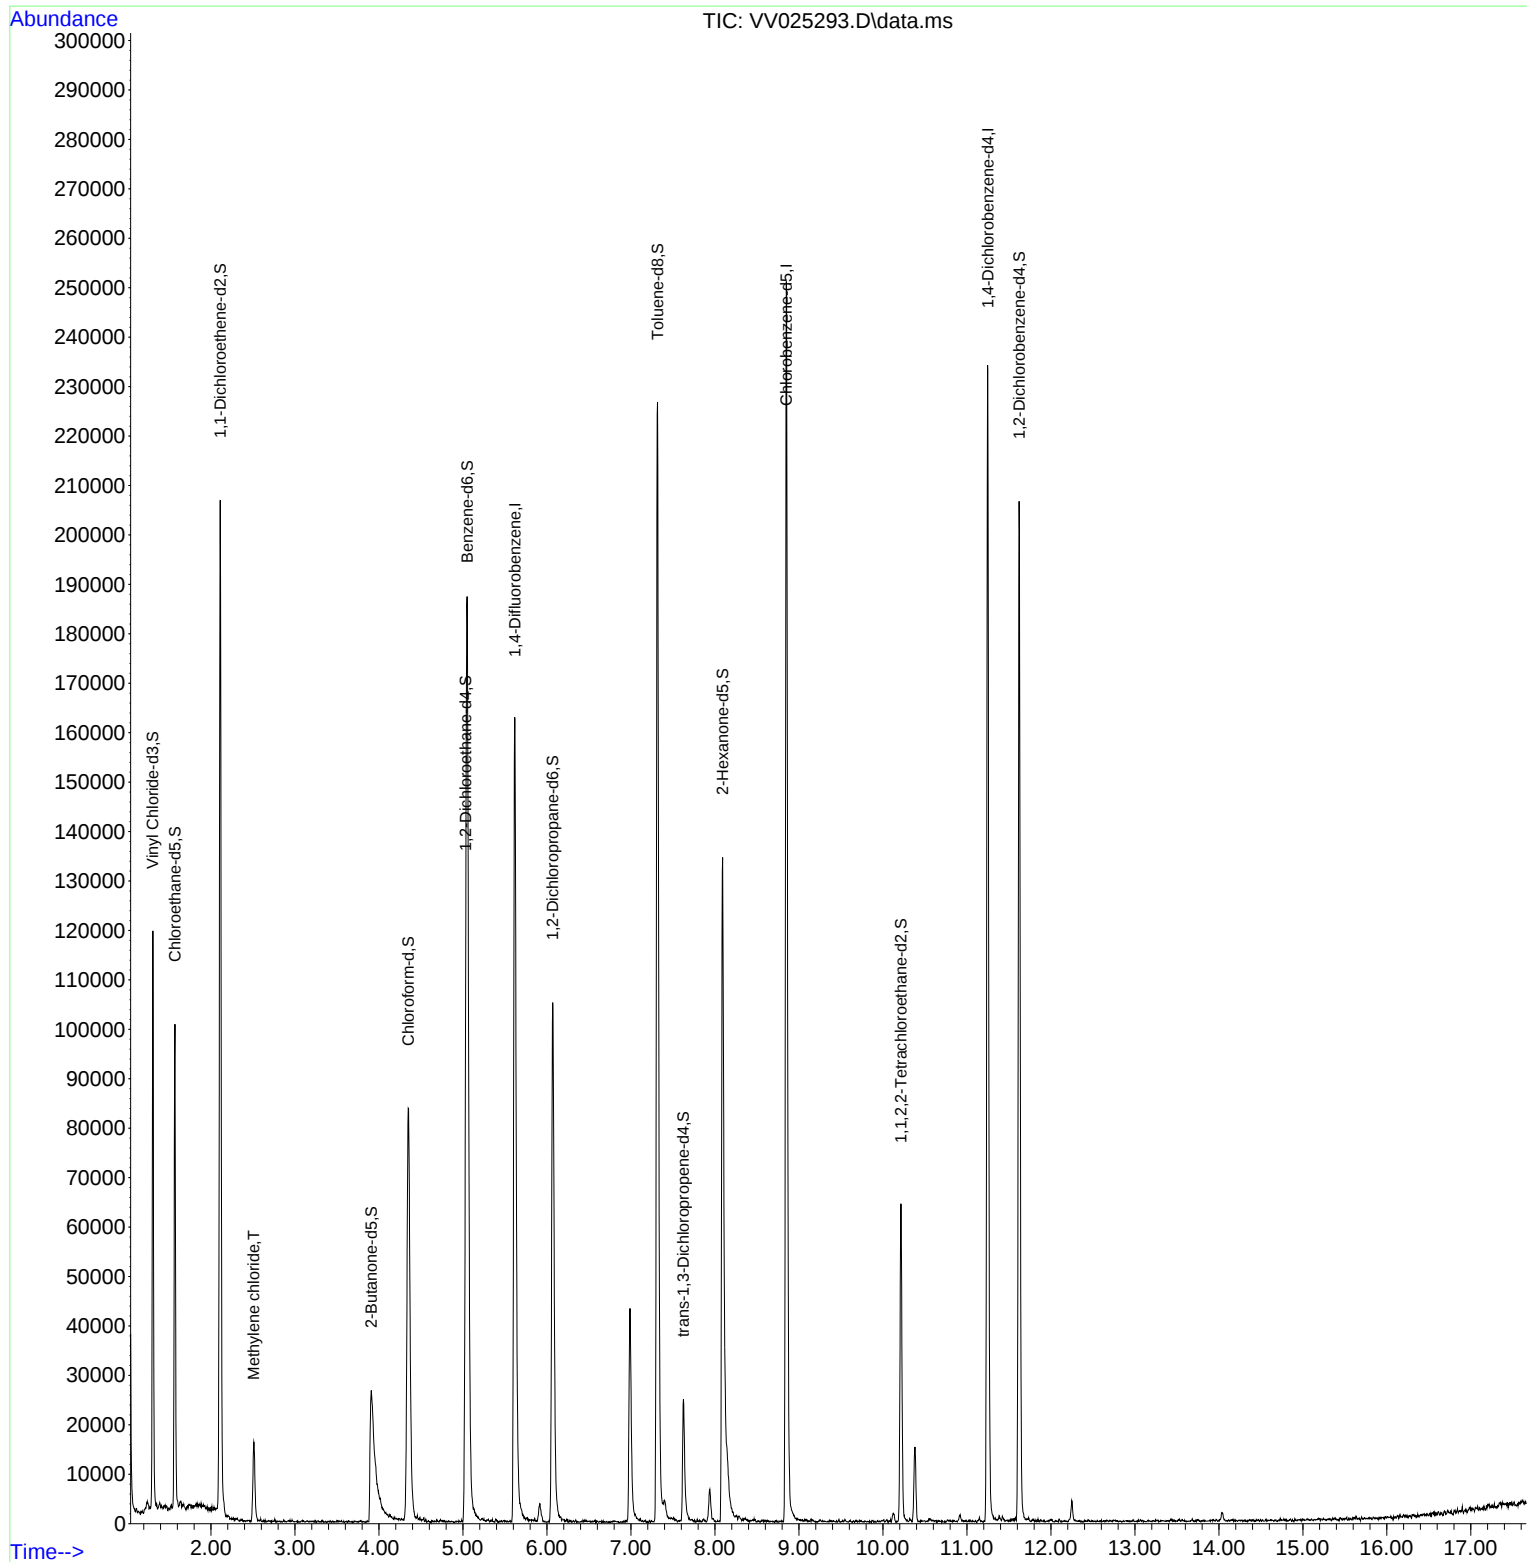

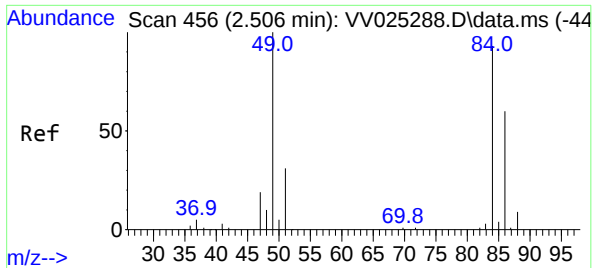

#16
Methylene chloride
Concen: 0.576 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025293.D
Acq: 29 Mar 2022 15:17

Instrument :
MSVOA_V
ClientSampleId :
EW6Q8

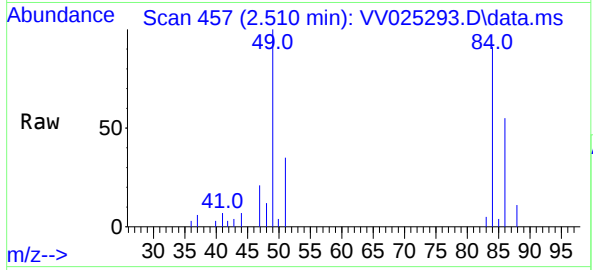

Tgt Ion: 84 Resp: 6766

Ion	Ratio	Lower	Upper
84	100		
86	60.7	43.5	80.7
49	110.4	74.5	138.3

