

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025296.D
 Acq On : 29 Mar 2022 16:27
 Operator : SY/MD
 Sample : N2165-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6N8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	73757	74720	17.59%	1.921%
2	1.568	156	164	173	rBV	77757	88806	20.90%	2.283%
3	2.108	322	332	355	rVB	140956	210728	49.60%	5.417%
4	2.510	449	457	468	rVB6	4030	6435	1.51%	0.165%
5	3.889	876	886	915	rBV	43851	141441	33.29%	3.636%
6	4.352	1014	1030	1063	rBV3	91365	300597	70.75%	7.727%
7	5.047	1230	1246	1272	rBV3	169124	424718	99.96%	10.917%
8	5.616	1412	1423	1444	rBV	166462	340794	80.21%	8.760%
9	5.915	1507	1516	1518	rBV5	3861	4903	1.15%	0.126%
10	6.069	1551	1564	1591	rBV	97133	204880	48.22%	5.266%
11	6.989	1838	1850	1872	rBV	40525	77496	18.24%	1.992%
12	7.317	1941	1952	1972	rBV	195856	343059	80.74%	8.818%
13	7.625	2039	2048	2066	rBV3	22343	40182	9.46%	1.033%
14	7.976	2147	2157	2176	rVB3	44637	78587	18.50%	2.020%
15	8.088	2182	2192	2223	rBV	164871	329690	77.59%	8.475%
16	8.850	2418	2429	2457	rBV	254970	424887	100.00%	10.922%
17	10.214	2842	2853	2870	rBV	69635	111557	26.26%	2.868%
18	10.384	2895	2906	2912	rBV4	6480	10251	2.41%	0.264%
19	11.246	3164	3174	3197	rBV	232566	365211	85.95%	9.388%
20	11.622	3279	3291	3308	rBV	190248	304525	71.67%	7.828%
21	12.246	3475	3485	3497	rBV3	4095	6833	1.61%	0.176%




Sum of corrected areas: 3890300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025296.D
Acq On : 29 Mar 2022 16:27
Operator : SY/MD
Sample : N2165-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

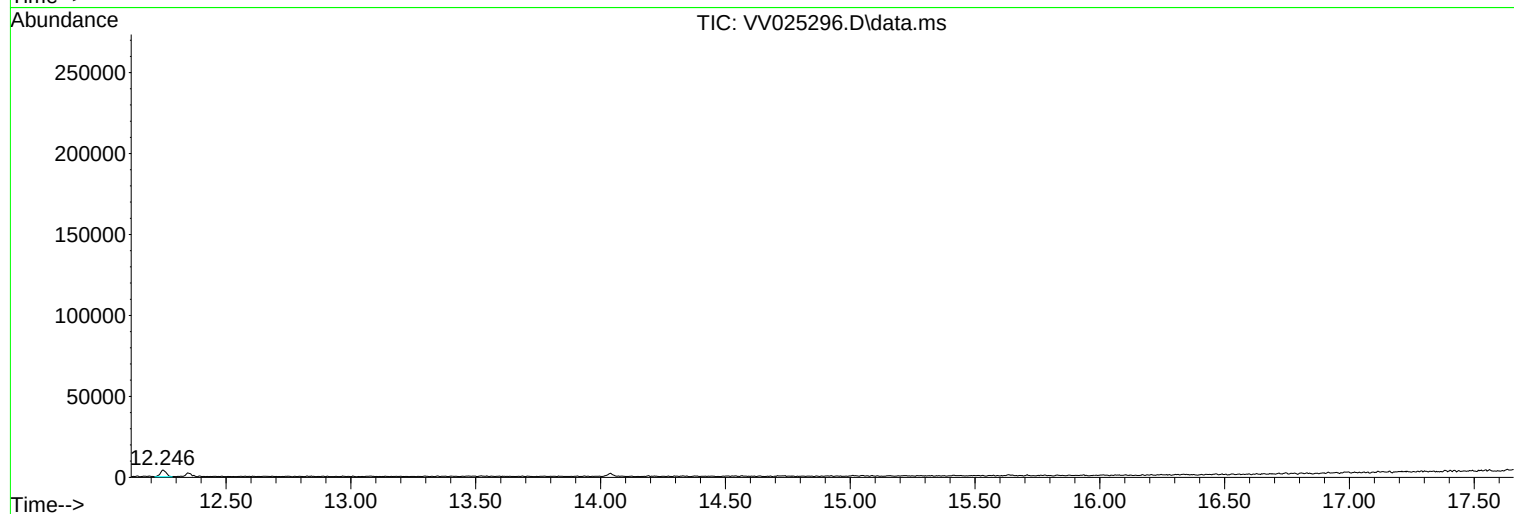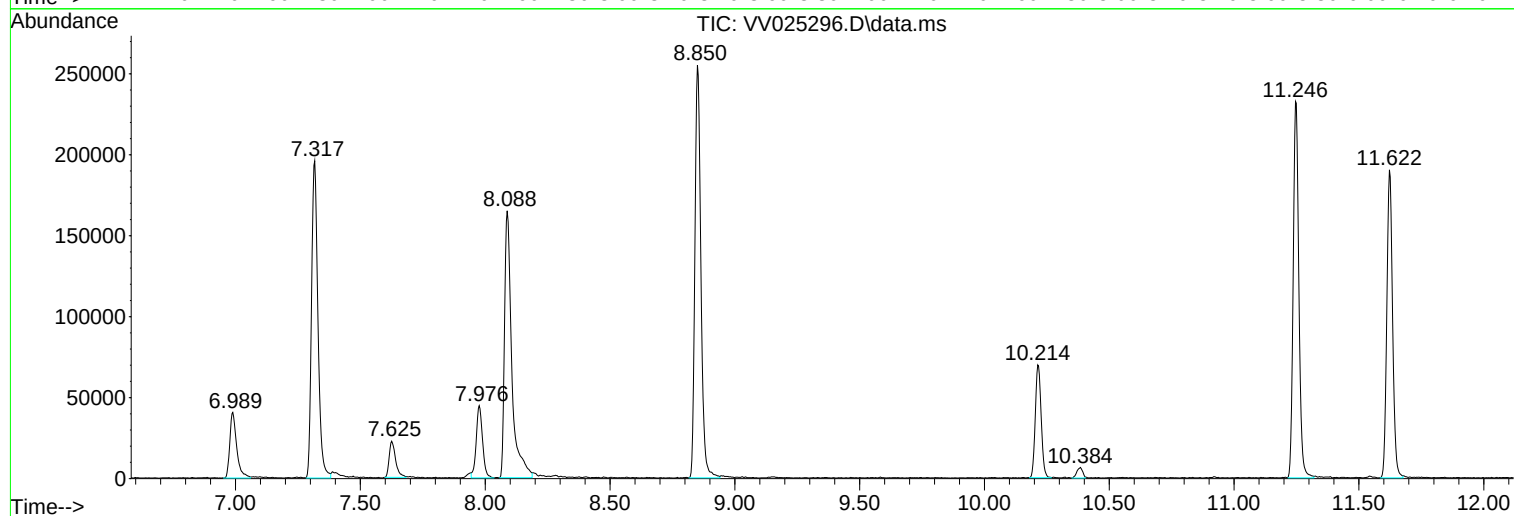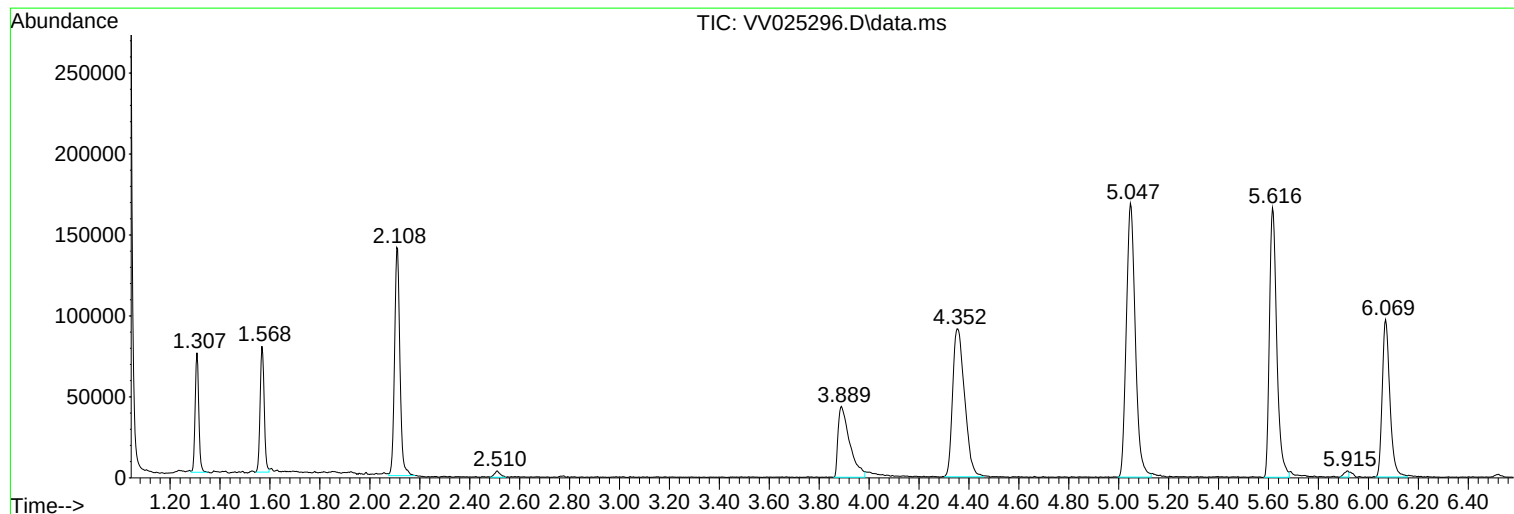

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025296.D
Acq On : 29 Mar 2022 16:27
Operator : SY/MD
Sample : N2165-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025296.D
Acq On : 29 Mar 2022 16:27
Operator : SY/MD
Sample : N2165-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc