

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025301.D
 Acq On : 29 Mar 2022 18:24
 Operator : SY/MD
 Sample : N2110-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	108581	110714	24.87%	2.960%
2	1.568	157	164	176	rBV	95935	109784	24.67%	2.935%
3	2.111	321	333	352	rVB	184448	274029	61.57%	7.326%
4	2.513	449	458	466	rBV3	3229	5562	1.25%	0.149%
5	3.889	877	886	924	rBV2	34821	105082	23.61%	2.809%
6	4.352	1013	1030	1058	rBV	78237	199922	44.92%	5.345%
7	5.047	1230	1246	1273	rBV2	176452	445083	100.00%	11.899%
8	5.616	1412	1423	1453	rBV	160393	328699	73.85%	8.788%
9	5.915	1506	1516	1525	rBV7	2702	5283	1.19%	0.141%
10	6.069	1551	1564	1586	rBV	99795	204192	45.88%	5.459%
11	6.989	1839	1850	1871	rBV2	41317	79144	17.78%	2.116%
12	7.317	1940	1952	1973	rBV	214915	383571	86.18%	10.255%
13	7.625	2038	2048	2068	rBV	22085	40598	9.12%	1.085%
14	7.937	2132	2145	2150	rBV4	3024	4604	1.03%	0.123%
15	7.979	2150	2158	2168	rVB5	11261	18895	4.25%	0.505%
16	8.088	2179	2192	2217	rBV	136935	263407	59.18%	7.042%
17	8.850	2418	2429	2446	rBV	247605	404104	90.79%	10.803%
18	10.214	2843	2853	2873	rVB	61501	98306	22.09%	2.628%
19	10.381	2899	2905	2916	rVB6	4127	6344	1.43%	0.170%
20	11.246	3161	3174	3194	rBV	224848	353590	79.44%	9.453%
21	11.622	3279	3291	3308	rBV	189285	299584	67.31%	8.009%




Sum of corrected areas: 3740497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025301.D
Acq On : 29 Mar 2022 18:24
Operator : SY/MD
Sample : N2110-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

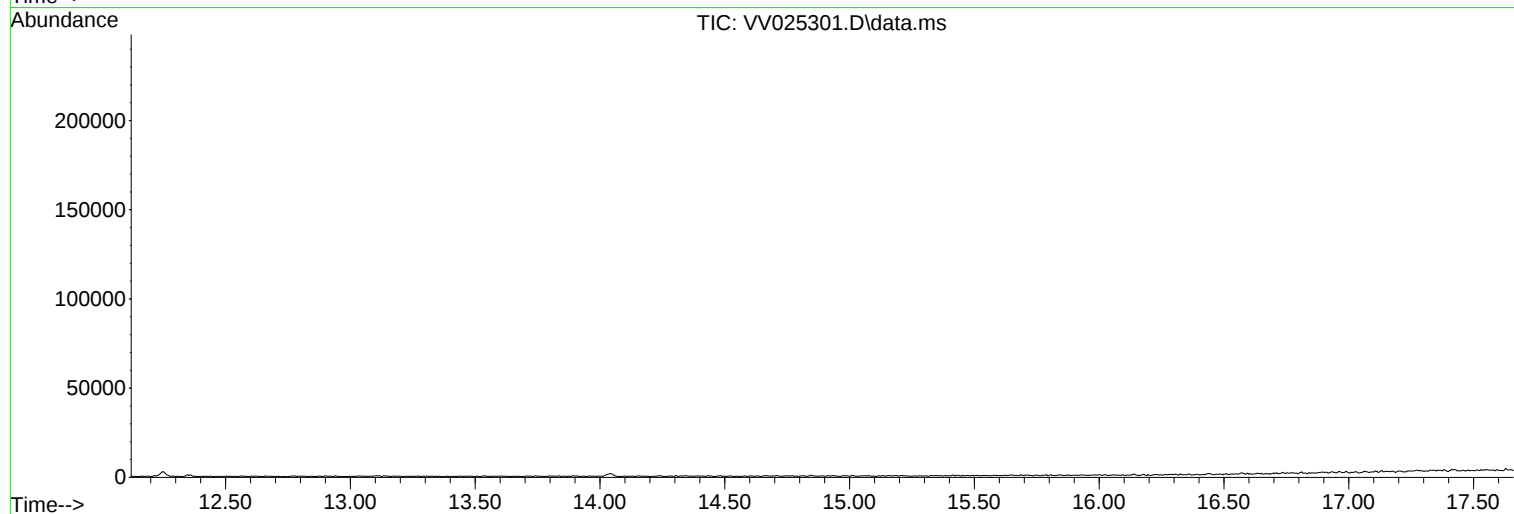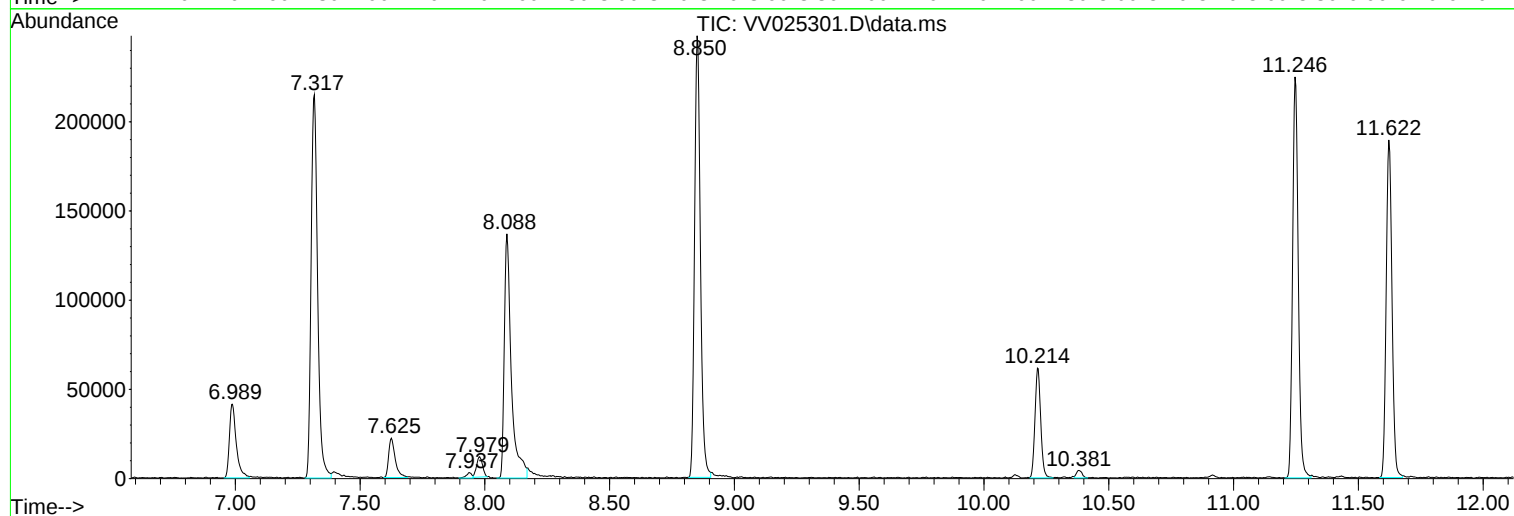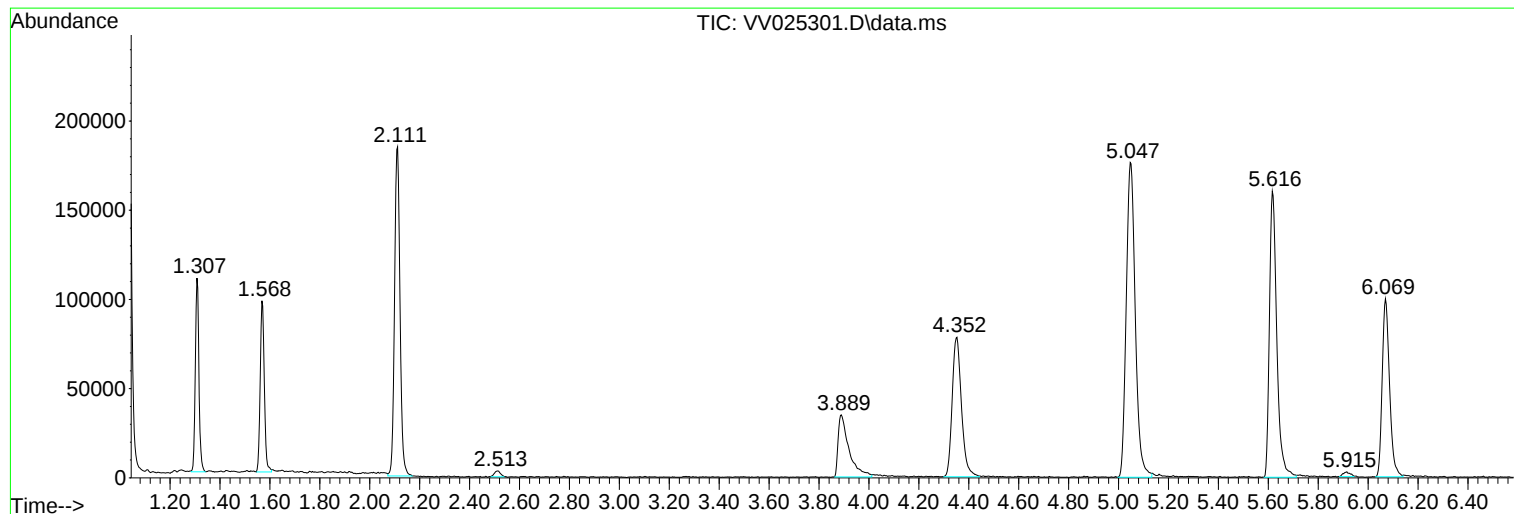

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025301.D
Acq On : 29 Mar 2022 18:24
Operator : SY/MD
Sample : N2110-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025301.D
Acq On : 29 Mar 2022 18:24
Operator : SY/MD
Sample : N2110-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc