

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025302.D
 Acq On : 29 Mar 2022 18:47
 Operator : SY/MD
 Sample : N2165-10MS
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6N7MS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	22	28	45	rVB	163525	152826	12.55%	0.690%
2	1.243	56	63	75	rBV	145358	156188	12.83%	0.706%
3	1.310	76	84	99	rVB2	231002	247079	20.29%	1.116%
4	1.523	142	150	158	rBV	161511	185655	15.25%	0.839%
5	1.587	158	170	182	rVB2	147551	247986	20.37%	1.120%
6	1.754	212	222	241	rVB	268874	357579	29.37%	1.616%
7	2.118	322	335	346	rBV3	567983	947910	77.84%	4.283%
8	2.179	347	354	379	rVB	47845	113688	9.34%	0.514%
9	2.298	379	391	406	rVB	155135	233264	19.16%	1.054%
10	2.439	428	435	446	rBV	12167	20667	1.70%	0.093%
11	2.510	446	457	473	rVB	151768	248771	20.43%	1.124%
12	2.764	523	536	561	rBV3	277534	543585	44.64%	2.456%
13	3.191	652	669	692	rBV	115306	245476	20.16%	1.109%
14	3.912	877	893	904	rBV3	145735	411628	33.80%	1.860%
15	3.970	905	911	942	rVB	61558	177227	14.55%	0.801%
16	4.249	982	998	1016	rBV	78534	194972	16.01%	0.881%
17	4.368	1016	1035	1062	rVB4	151058	500402	41.09%	2.261%
18	4.609	1091	1110	1120	rBV2	133701	333270	27.37%	1.506%
19	4.677	1121	1131	1153	rVB	172594	426761	35.05%	1.928%
20	4.828	1158	1178	1197	rBV	128693	302295	24.83%	1.366%
21	5.050	1231	1247	1254	rBV3	171421	405037	33.26%	1.830%
22	5.098	1255	1262	1303	rVB2	260539	708755	58.20%	3.202%
23	5.616	1412	1423	1457	rBV	179608	370774	30.45%	1.675%
24	5.915	1502	1516	1539	rBV2	197371	399147	32.78%	1.803%
25	6.069	1553	1564	1573	rBV	95844	193672	15.90%	0.875%
26	6.130	1573	1583	1590	rVV	225614	457515	37.57%	2.067%
27	6.172	1591	1596	1619	rVB	159539	294631	24.20%	1.331%
28	6.510	1686	1701	1720	rBV	121357	229793	18.87%	1.038%
29	6.989	1839	1850	1854	rBV2	47319	72751	5.97%	0.329%
30	7.027	1855	1862	1883	rVB2	127411	228325	18.75%	1.032%
31	7.223	1912	1923	1941	rBV	452474	793491	65.16%	3.585%
32	7.317	1941	1952	1964	rVV	206460	379044	31.13%	1.713%
33	7.387	1964	1974	1999	rVB	392704	678072	55.68%	3.064%
34	7.651	2038	2056	2075	rBV3	108870	236575	19.43%	1.069%
35	7.838	2101	2114	2133	rBV2	142831	245280	20.14%	1.108%
36	7.976	2141	2157	2173	rBV	248482	421155	34.59%	1.903%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025302.D
 Acq On : 29 Mar 2022 18:47
 Operator : SY/MD
 Sample : N2165-10MS
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6N7MS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

37	8.088	2181	2192	2200	rBV	196066	329358	27.05%	1.488%
38	8.137	2200	2207	2229	rVV	341267	575895	47.29%	2.602%
39	8.246	2229	2241	2262	rVB	94276	171276	14.07%	0.774%
40	8.352	2262	2274	2291	rBV	62700	106917	8.78%	0.483%
41	8.850	2419	2429	2433	rBV	291490	437684	35.94%	1.977%
42	8.879	2434	2438	2462	rVB	336603	507498	41.68%	2.293%
43	9.011	2467	2479	2504	rVV	435214	674915	55.43%	3.049%
44	9.137	2506	2518	2540	rBV	397809	652182	53.56%	2.947%
45	9.551	2632	2647	2677	rBV5	554166	1217695	100.00%	5.502%
46	9.728	2692	2702	2718	rVB2	47047	77878	6.40%	0.352%
47	9.931	2749	2765	2788	rBV	450755	715140	58.73%	3.231%
48	10.217	2837	2854	2856	rBV2	80941	108465	8.91%	0.490%
49	10.272	2866	2871	2887	rVB	94133	141524	11.62%	0.639%
50	10.538	2941	2954	2971	rBV	228284	351197	28.84%	1.587%
51	10.911	3058	3070	3087	rBV	417454	630713	51.80%	2.850%
52	11.178	3140	3153	3165	rBV	340426	530693	43.58%	2.398%
53	11.249	3165	3175	3177	rBV	336516	426913	35.06%	1.929%
54	11.635	3279	3295	3315	rBV2	359398	817739	67.15%	3.695%
55	12.342	3507	3515	3526	rBV6	13310	20833	1.71%	0.094%
56	12.426	3530	3541	3554	rVV3	25603	42012	3.45%	0.190%
57	12.641	3596	3608	3624	rBV	306566	477379	39.20%	2.157%
58	13.259	3788	3800	3816	rBV	241982	374529	30.76%	1.692%
59	13.500	3864	3875	3893	rBV	151119	235379	19.33%	1.063%
60	13.741	3938	3950	3973	rVB	226613	348143	28.59%	1.573%




Sum of corrected areas: 22133203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025302.D
Acq On : 29 Mar 2022 18:47
Operator : SY/MD
Sample : N2165-10MS
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N7MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

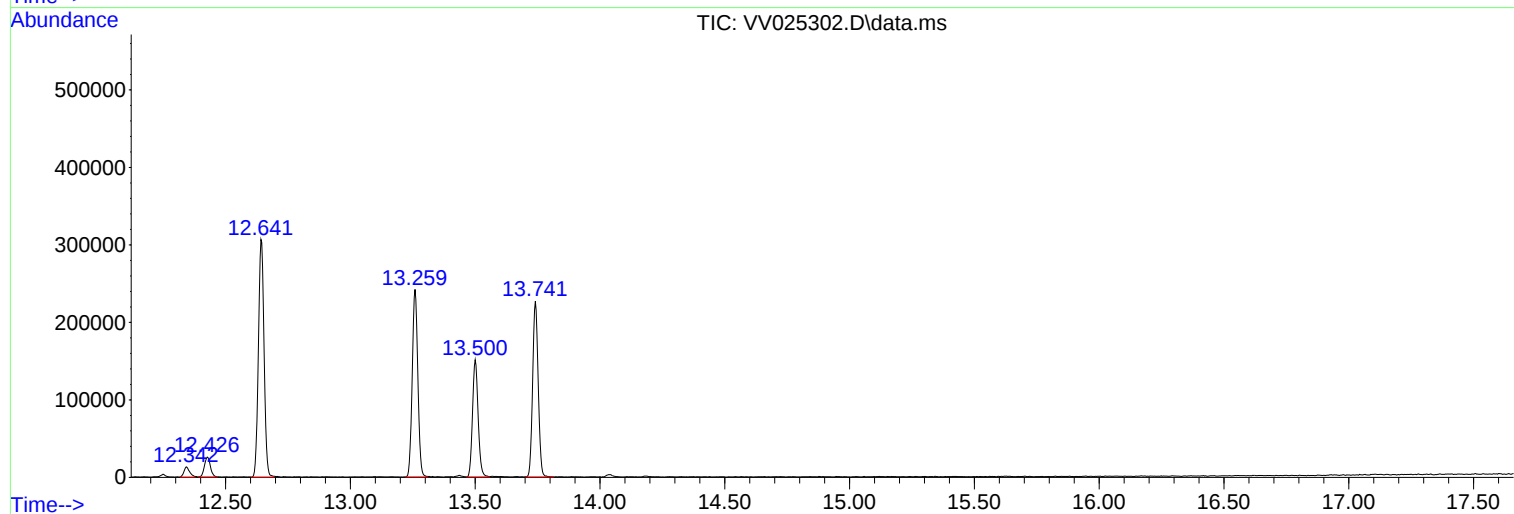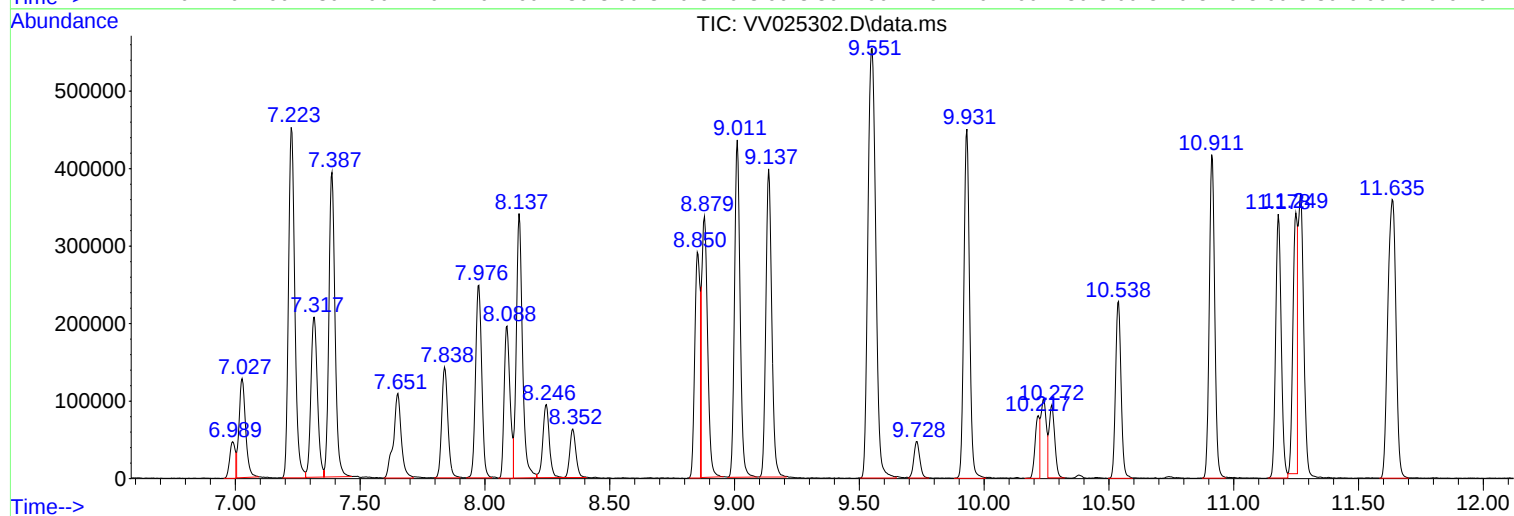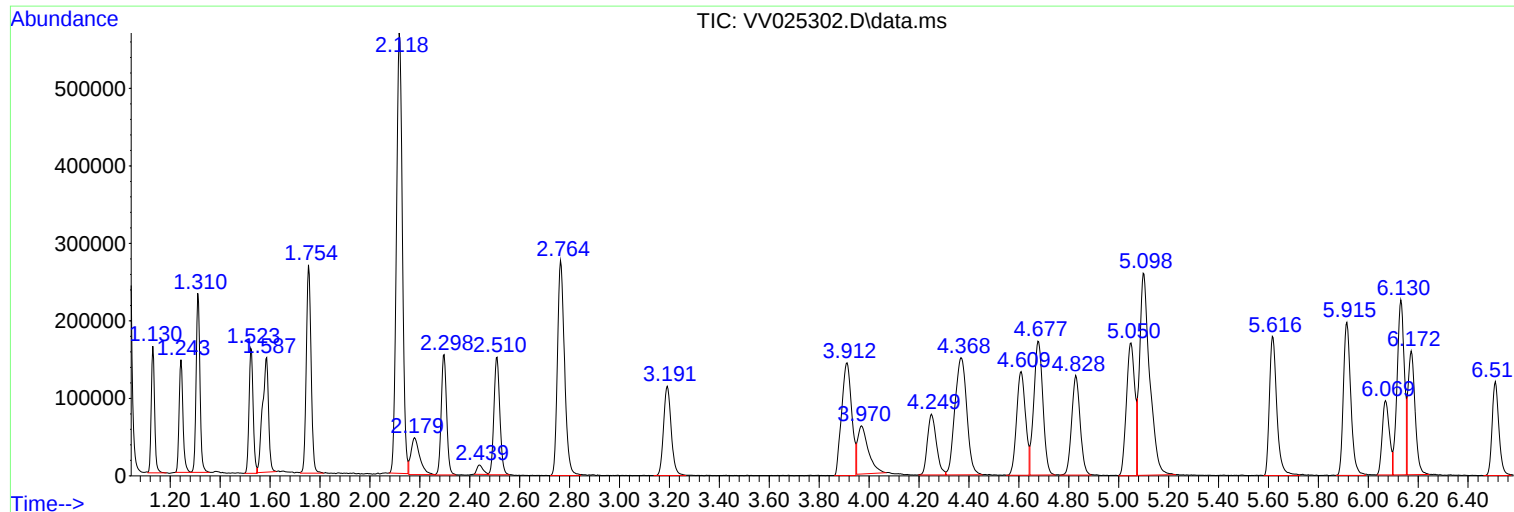

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025302.D
Acq On : 29 Mar 2022 18:47
Operator : SY/MD
Sample : N2165-10MS
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N7MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025302.D
Acq On : 29 Mar 2022 18:47
Operator : SY/MD
Sample : N2165-10MS
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N7MS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc