

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025303.D
 Acq On : 29 Mar 2022 19:11
 Operator : SY/MD
 Sample : N2165-11MSD
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6N7MSD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	22	28	44	rVB	155344	139027	13.02%	0.693%
2	1.243	56	63	76	rBV	133277	143705	13.45%	0.717%
3	1.311	76	84	100	rVB2	213354	233375	21.85%	1.164%
4	1.523	142	150	158	rBV	146694	170028	15.92%	0.848%
5	1.587	158	170	180	rVB2	126600	218748	20.48%	1.091%
6	1.754	213	222	236	rVB	240182	315221	29.51%	1.572%
7	2.118	322	335	347	rBV3	511264	858786	80.40%	4.283%
8	2.182	347	355	379	rVV	39622	101865	9.54%	0.508%
9	2.298	380	391	410	rVB	141511	213940	20.03%	1.067%
10	2.439	427	435	445	rBV	10705	20045	1.88%	0.100%
11	2.507	446	456	477	rVB	133588	221738	20.76%	1.106%
12	2.764	519	536	558	rBV2	246105	483901	45.30%	2.414%
13	3.191	652	669	692	rBV	101250	217891	20.40%	1.087%
14	3.912	876	893	905	rBV3	134124	382063	35.77%	1.906%
15	3.973	906	912	946	rVB	53297	157249	14.72%	0.784%
16	4.249	984	998	1015	rBV3	70018	173884	16.28%	0.867%
17	4.368	1017	1035	1062	rVB4	135821	457654	42.84%	2.283%
18	4.609	1090	1110	1121	rBV2	120027	304876	28.54%	1.521%
19	4.677	1121	1131	1151	rVB2	152641	378692	35.45%	1.889%
20	4.828	1161	1178	1199	rBV2	111546	265953	24.90%	1.326%
21	5.050	1232	1247	1254	rBV2	164834	388659	36.38%	1.939%
22	5.098	1255	1262	1292	rVB2	227610	621627	58.19%	3.100%
23	5.616	1412	1423	1448	rBV	170533	349743	32.74%	1.744%
24	5.915	1503	1516	1536	rBV	175036	351794	32.93%	1.755%
25	6.069	1552	1564	1573	rBV2	94712	190441	17.83%	0.950%
26	6.130	1573	1583	1590	rVV2	201557	414905	38.84%	2.069%
27	6.172	1591	1596	1617	rVB	144754	262481	24.57%	1.309%
28	6.510	1689	1701	1721	rBV	106451	202747	18.98%	1.011%
29	6.989	1840	1850	1855	rBV	45677	75592	7.08%	0.377%
30	7.027	1855	1862	1883	rVB	113894	206883	19.37%	1.032%
31	7.223	1909	1923	1941	rBV	398140	704241	65.93%	3.513%
32	7.317	1941	1952	1964	rVV	205766	371261	34.76%	1.852%
33	7.387	1964	1974	2000	rVB	338435	599212	56.10%	2.989%
34	7.651	2038	2056	2075	rBV2	94973	212185	19.86%	1.058%
35	7.838	2102	2114	2134	rBV2	127006	217735	20.38%	1.086%
36	7.976	2144	2157	2175	rVB	222683	376825	35.28%	1.879%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032922\
 Data File : VW025303.D
 Acq On : 29 Mar 2022 19:11
 Operator : SY/MD
 Sample : N2165-11MSD
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6N7MSD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

37	8.088	2181	2192	2200	rBV	192661	326045	30.52%	1.626%
38	8.137	2200	2207	2230	rVV	302439	512904	48.02%	2.558%
39	8.243	2230	2240	2254	rVB	85591	145957	13.66%	0.728%
40	8.352	2263	2274	2289	rBV	56029	93449	8.75%	0.466%
41	8.850	2415	2429	2433	rBV	278795	411389	38.51%	2.052%
42	8.879	2434	2438	2457	rVB	300375	450826	42.20%	2.249%
43	9.011	2466	2479	2505	rVB	375090	596430	55.83%	2.975%
44	9.137	2507	2518	2539	rVV	350656	577370	54.05%	2.880%
45	9.548	2631	2646	2668	rBV3	477188	1068203	100.00%	5.328%
46	9.728	2692	2702	2719	rBV	42973	71650	6.71%	0.357%
47	9.931	2750	2765	2789	rBV	408282	638589	59.78%	3.185%
48	10.217	2842	2854	2856	rBV2	77982	103302	9.67%	0.515%
49	10.272	2867	2871	2888	rVB	81824	117654	11.01%	0.587%
50	10.538	2943	2954	2970	rBV	204744	311458	29.16%	1.553%
51	10.911	3058	3070	3089	rBV	364827	552256	51.70%	2.754%
52	11.178	3138	3153	3165	rBV	302976	474233	44.40%	2.365%
53	11.249	3165	3175	3178	rBV	310962	451364	42.25%	2.251%
54	11.635	3279	3295	3318	rBV2	330394	762991	71.43%	3.806%
55	12.342	3508	3515	3526	rBV3	13541	20931	1.96%	0.104%
56	12.426	3531	3541	3559	rVB2	24155	38670	3.62%	0.193%
57	12.641	3596	3608	3625	rBV	284947	438812	41.08%	2.189%
58	13.259	3789	3800	3819	rBV	226539	346964	32.48%	1.731%
59	13.500	3865	3875	3894	rBV	137615	215465	20.17%	1.075%
60	13.741	3938	3950	3968	rBV	204306	317564	29.73%	1.584%




Sum of corrected areas: 20049448

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025303.D
Acq On : 29 Mar 2022 19:11
Operator : SY/MD
Sample : N2165-11MSD
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N7MSD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

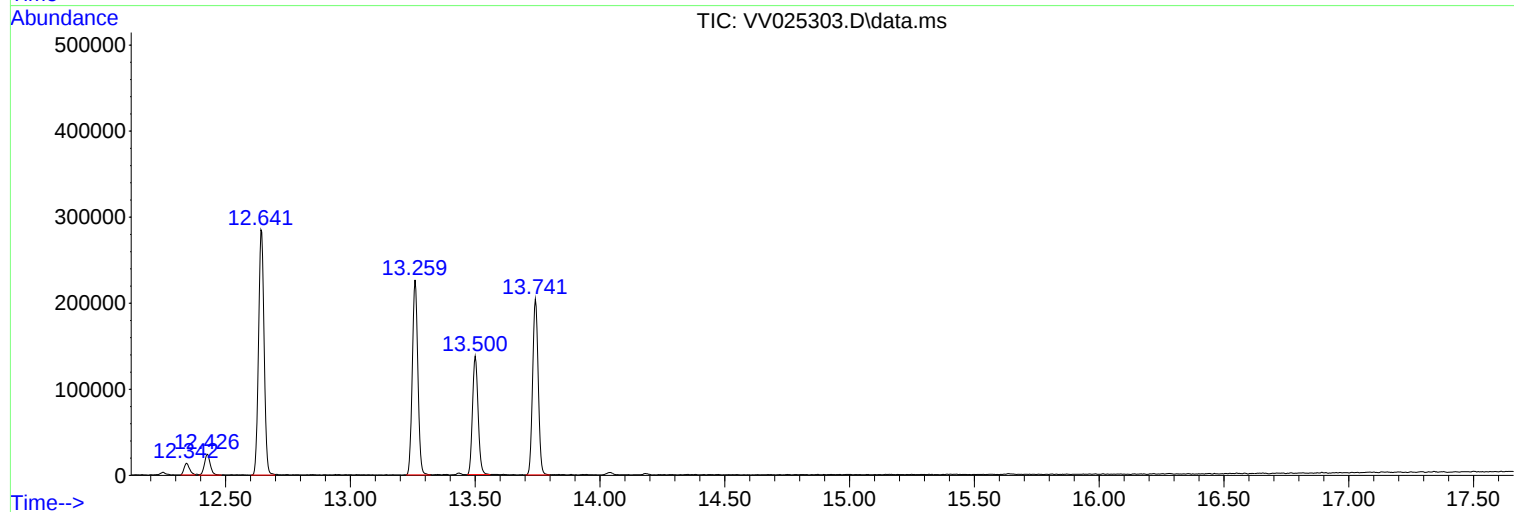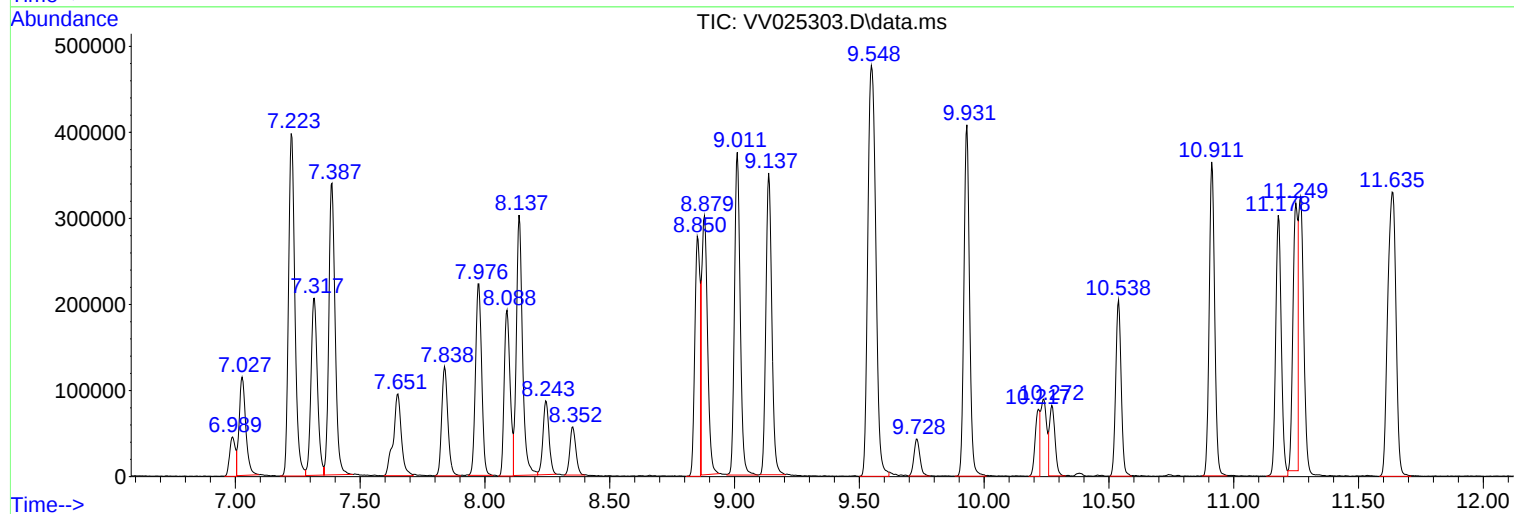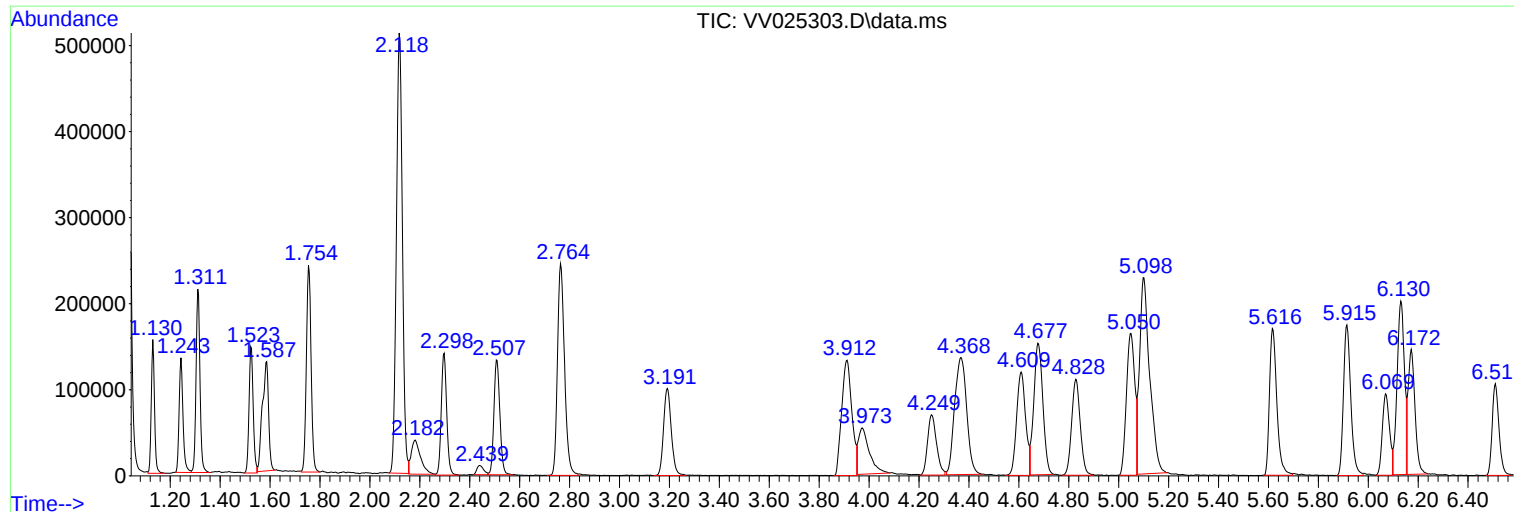

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025303.D
Acq On : 29 Mar 2022 19:11
Operator : SY/MD
Sample : N2165-11MSD
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N7MSD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
Data File : VV025303.D
Acq On : 29 Mar 2022 19:11
Operator : SY/MD
Sample : N2165-11MSD
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6N7MSD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc