
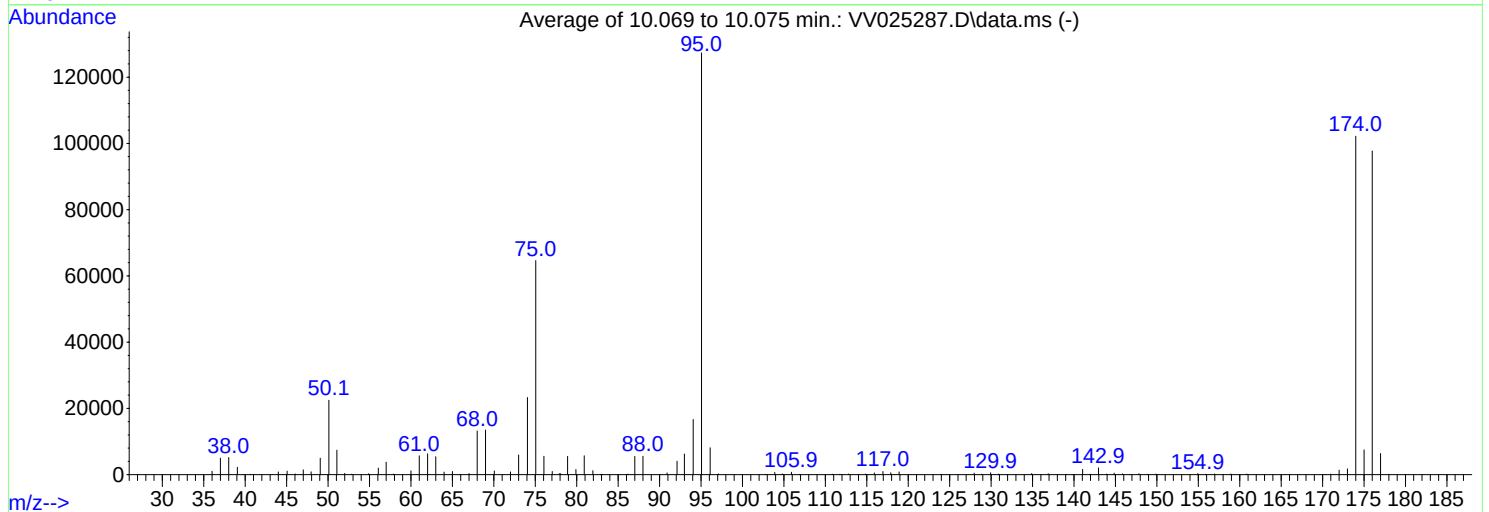


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032922\
 Data File : VV025287.D
 Acq On : 29 Mar 2022 09:01
 Operator : SY/MD
 Sample : BFB290
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB290

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Apr 01 01:30:42 2022

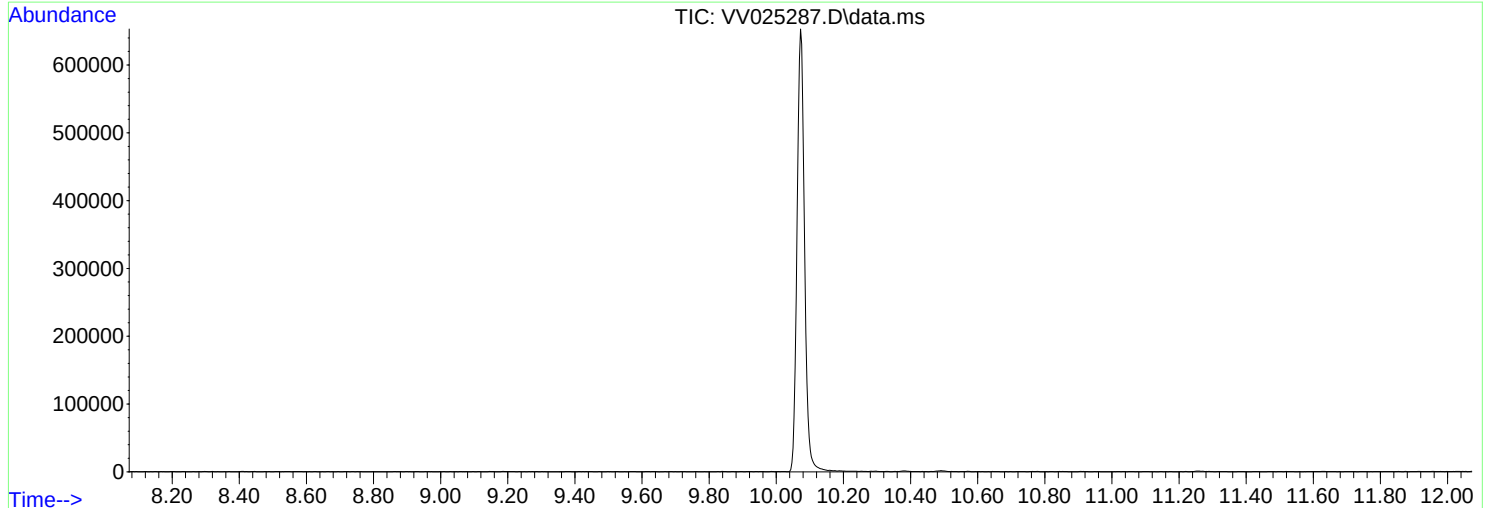

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	22485	PASS
75	95	30	80	50.8	64653	PASS
95	95	100	100	100.0	127331	PASS
96	95	5	9	6.4	8119	PASS
173	174	0.00	2	1.7	1762	PASS
174	95	50	120	80.2	102152	PASS
175	174	5	9	7.3	7490	PASS
176	174	95	105	95.7	97712	PASS
177	176	5	10	6.5	6391	PASS

m/z	Abundance
39.80	151.0
44.00	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	920.0
37.00	4817.0
38.00	4991.0
39.10	2141.0
39.90	226.0
40.70	103.0
44.00	1060.0
45.10	1011.0
46.10	242.0
47.00	1458.0
48.00	893.0
49.00	4912.0
50.10	22032.0
51.10	7240.0
52.00	385.0
52.80	115.0
54.90	313.0
56.10	1951.0
57.00	3675.0
57.90	235.0
60.00	1224.0
61.00	5664.0
62.00	6154.0
63.00	5361.0
64.00	841.0
65.00	1085.0
65.90	108.0
66.90	314.0
68.00	12578.0
69.00	13159.0
70.10	1057.0
72.00	788.0
73.00	5915.0
74.10	22768.0
75.00	63592.0
76.10	5347.0
77.00	821.0
77.90	525.0
78.90	5269.0
79.90	1542.0
80.90	5588.0
81.90	1240.0
82.80	112.0
86.20	178.0
87.00	5398.0
88.00	5138.0
90.90	512.0
92.10	4059.0
93.00	5985.0
94.00	16166.0
95.10	123152.0
96.10	8125.0
97.20	262.0
102.80	109.0
103.90	677.0
104.80	248.0
105.90	684.0
106.90	110.0
110.80	140.0
111.70	133.0
112.80	174.0
114.80	202.0
115.90	427.0
116.90	987.0
117.90	557.0
118.90	747.0
128.00	411.0
128.90	156.0
130.00	492.0
130.90	219.0
131.90	107.0
134.90	352.0
136.90	325.0
139.10	108.0
139.80	106.0
141.10	1426.0
141.90	203.0
142.90	2014.0
143.90	235.0
144.80	478.0
145.90	261.0
147.80	263.0
148.90	143.0
149.90	189.0
154.90	314.0
155.90	115.0
157.00	285.0
158.00	105.0
159.00	191.0
160.80	184.0
171.00	237.0
172.00	1349.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

173.00	1594.0
174.00	96440.0
175.00	7289.0
176.00	92208.0
177.00	6080.0
178.00	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	1083.0
37.00	5090.0
38.00	5339.0
39.10	2292.0
39.90	196.0
40.70	107.0
44.00	1048.0
45.10	1052.0
46.10	228.0
47.00	1533.0
48.00	905.0
49.10	5242.0
50.10	23344.0
51.10	7708.0
52.00	428.0
52.80	126.0
54.90	313.0
56.00	2042.0
57.00	3885.0
57.90	198.0
60.00	1194.0
61.00	5805.0
62.00	6485.0
63.00	5579.0
64.00	826.0
65.00	972.0
67.00	382.0
68.00	13642.0
69.00	13940.0
70.00	1148.0
72.00	847.0
73.00	6105.0
74.00	24040.0
75.10	67048.0
76.10	5682.0
77.10	984.0
77.90	472.0
78.10	474.0
78.90	5728.0
79.90	1632.0
80.90	6003.0
82.00	1272.0
82.80	117.0
86.20	240.0
87.00	5682.0
88.00	5760.0
90.90	545.0
92.10	4233.0
93.00	6506.0
94.10	17328.0
95.00	132032.0
96.10	8270.0
97.10	235.0
102.70	128.0
103.90	719.0
104.80	268.0
105.90	764.0
106.90	123.0
110.90	182.0
111.80	144.0
112.80	194.0
114.80	199.0
115.90	562.0
116.90	1003.0
117.90	570.0
118.90	837.0
123.90	100.0
127.90	498.0
128.90	162.0
130.00	580.0
130.90	206.0
134.90	374.0
136.90	325.0
141.00	1665.0
142.00	202.0
143.00	2136.0
144.00	218.0
144.80	478.0
145.90	240.0
146.70	101.0
147.80	313.0
148.90	127.0
149.90	179.0
155.00	335.0
155.90	138.0
157.00	276.0
158.00	130.0
159.00	234.0
160.90	212.0
171.00	232.0
172.00	1406.0
173.00	1836.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

174.00	105696.0
175.00	7765.0
176.00	101096.0
177.00	6577.0
178.00	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	1101.0
37.00	4987.0
38.00	5170.0
39.00	2204.0
39.80	188.0
40.50	123.0
44.00	980.0
45.00	1101.0
46.00	185.0
47.00	1376.0
47.90	796.0
49.00	4845.0
50.10	22080.0
51.00	7178.0
52.00	433.0
52.90	143.0
54.90	296.0
56.00	1991.0
57.00	3774.0
57.90	133.0
60.00	1098.0
61.00	5615.0
62.00	6234.0
63.00	5271.0
64.00	724.0
65.00	873.0
67.10	397.0
68.00	13323.0
69.00	13343.0
70.00	1171.0
72.00	773.0
73.00	5773.0
74.10	23056.0
75.10	63320.0
76.00	5623.0
77.10	1059.0
78.00	475.0
78.90	5511.0
79.90	1519.0
80.90	5489.0
81.90	1158.0
82.90	111.0
83.10	110.0
86.20	230.0
87.00	5450.0
88.00	5727.0
90.90	533.0
92.10	3960.0
93.00	6245.0
94.00	16504.0
95.00	126808.0
96.10	7961.0
97.00	221.0
102.70	135.0
103.90	687.0
104.80	254.0
105.90	789.0
106.90	117.0
110.90	186.0
111.80	155.0
112.80	195.0
114.90	180.0
115.90	604.0
117.00	937.0
117.90	580.0
118.90	849.0
124.00	113.0
127.90	548.0
128.80	203.0
129.90	643.0
130.90	180.0
134.90	308.0
136.90	277.0
141.00	1690.0
142.90	1958.0
144.00	173.0
144.90	442.0
145.80	207.0
147.90	334.0
148.90	105.0
149.90	160.0
155.00	343.0
155.90	117.0
156.90	199.0
158.00	104.0
158.90	190.0
160.90	208.0
170.30	106.0
171.00	198.0
172.00	1325.0
173.00	1857.0
174.00	104320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

175.00	7417.0
176.00	99832.0
177.00	6515.0
178.00	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290