

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034909.D
 Acq On : 29 Mar 2024 16:37
 Operator : SY/MD
 Sample : P1934-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1


Instrument :
 MSVOA_V
 ClientSampleId :
 C0R40

Quant Time: Mar 30 02:15:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 29 00:23:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	320576	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	309698	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	143077	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	134557	43.462	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.920%	
7) Chloroethane-d5	1.532	69	117635	43.746	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	87.500%	
11) 1,1-Dichloroethene-d2	2.060	65	62943	46.380	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.760%	
21) 2-Butanone-d5	3.789	46	143734	78.280	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	78.280%	
24) Chloroform-d	4.249	84	227581	43.721	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.440%	
26) 1,2-Dichloroethane-d4	4.941	65	146558	44.347	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.700%	
32) Benzene-d6	4.960	84	461165	44.330	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.660%	
36) 1,2-Dichloropropane-d6	5.989	67	147217	44.565	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	89.120%	
41) Toluene-d8	7.243	98	402222	42.933	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	85.860%	
43) trans-1,3-Dichloroprop...	7.555	79	61572	38.340	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	76.680%	
47) 2-Hexanone-d5	8.024	63	88577	70.920	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	70.920%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	191225	42.036	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	84.080%	
66) 1,2-Dichlorobenzene-d4	11.561	152	145402	45.263	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.520%	
Target Compounds						
					Qvalue	
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	1763	0.701	ug/L #	22
48) 2-Hexanone	8.085	43	17399	5.741	ug/L #	78





(#) = qualifier out of range (m) = manual integration (+) = signals summed

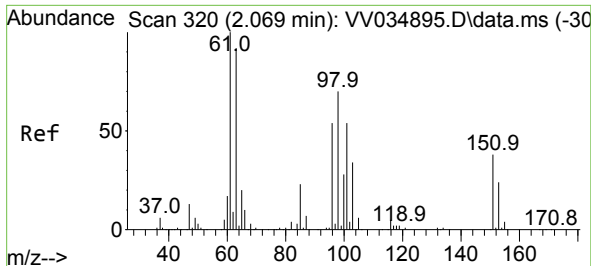

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.701 ug/L
RT: 2.060 min Scan# 317
Delta R.T. -0.010 min
Lab File: VV034909.D
Acq: 29 Mar 2024 16:37

Instrument :
MSVOA_V
ClientSampleId :
C0R40

Tgt Ion:101 Resp: 1763
Ion Ratio Lower Upper
101 100
85 0.0 35.3 52.9#
151 0.0 55.0 82.4#

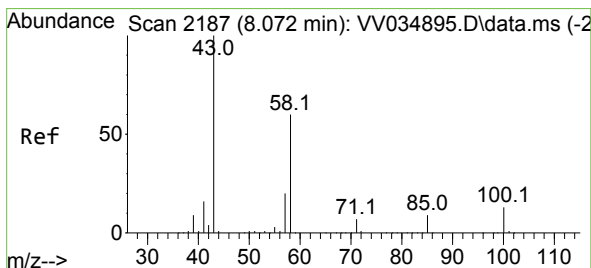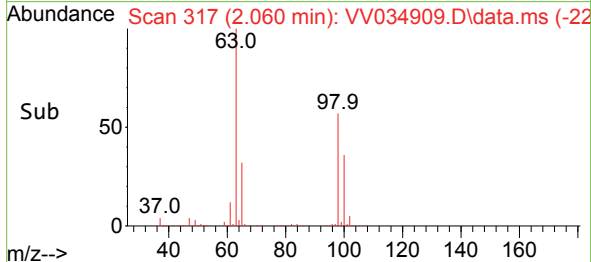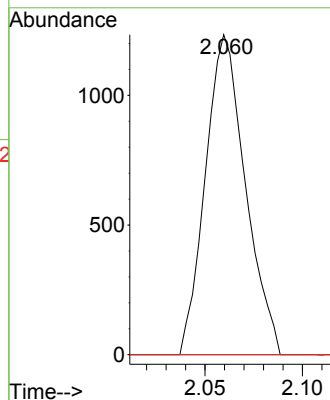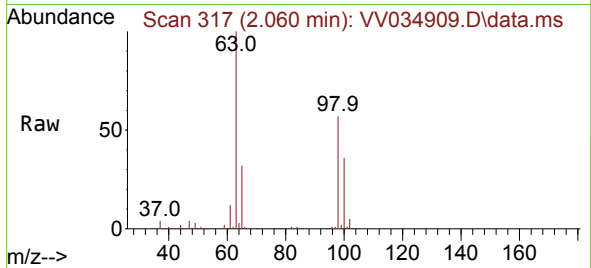

#48
2-Hexanone
Concen: 5.741 ug/L
RT: 8.085 min Scan# 2191
Delta R.T. 0.013 min
Lab File: VV034909.D
Acq: 29 Mar 2024 16:37

Tgt Ion: 43 Resp: 17399
Ion Ratio Lower Upper
43 100
58 38.4 45.4 68.2#
57 12.8 16.2 24.4#
100 4.9 10.1 15.1#

