

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034897.D
 Acq On : 29 Mar 2024 09:57
 Operator : SY/MD
 Sample : P1856-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	96	rVB	238011	252147	16.69%	2.235%
2	1.532	147	153	170	rVB	219835	259077	17.14%	2.296%
3	2.063	308	318	348	rVB	399758	601762	39.82%	5.333%
4	2.246	371	375	378	rBV2	1020	791	0.05%	0.007%
5	2.281	383	386	387	rBV2	497	298	0.02%	0.003%
6	2.420	424	429	432	rBV2	786	596	0.04%	0.005%
7	2.439	432	435	436	rBV2	736	374	0.02%	0.003%
8	2.529	458	463	465	rBV	367	424	0.03%	0.004%
9	2.690	509	513	514	rBV	357	247	0.02%	0.002%
10	2.716	519	521	523	rBV2	313	142	0.01%	0.001%
11	2.761	534	535	538	rBV2	276	163	0.01%	0.001%
12	2.851	560	563	566	rVB	291	135	0.01%	0.001%
13	2.912	579	582	585	rVB	246	132	0.01%	0.001%
14	2.931	585	588	589	rBV	410	243	0.02%	0.002%
15	2.995	605	608	610	rVB2	584	251	0.02%	0.002%
16	3.011	610	613	615	rBV	182	116	0.01%	0.001%
17	3.114	643	645	651	rVB3	432	312	0.02%	0.003%
18	3.159	656	659	663	rVB3	386	284	0.02%	0.003%
19	3.182	663	666	669	rVB2	390	279	0.02%	0.002%
20	3.259	684	690	694	rBV3	584	541	0.04%	0.005%
21	3.288	694	699	703	rBV3	339	385	0.03%	0.003%
22	3.346	713	717	725	rBV3	568	615	0.04%	0.005%
23	3.397	730	733	737	rBV2	391	345	0.02%	0.003%
24	3.433	740	744	746	rBV2	452	267	0.02%	0.002%
25	3.474	754	757	761	rVB	371	305	0.02%	0.003%
26	3.500	761	765	767	rBV2	467	275	0.02%	0.002%
27	3.577	786	789	790	rBV	362	156	0.01%	0.001%
28	3.683	819	822	827	rBV2	500	390	0.03%	0.003%
29	3.706	827	829	831	rBV	332	188	0.01%	0.002%
30	3.748	837	842	845	rVB2	285	207	0.01%	0.002%
31	3.789	847	855	889	rBV	86535	259251	17.16%	2.298%
32	4.249	982	998	1034	rBV2	229035	597496	39.54%	5.295%
33	4.641	1118	1120	1122	rVB	571	228	0.02%	0.002%
34	4.661	1122	1126	1129	rBV3	591	457	0.03%	0.004%
35	4.687	1129	1134	1136	rBV	354	381	0.03%	0.003%
36	4.719	1140	1144	1145	rBV	493	338	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034897.D
 Acq On : 29 Mar 2024 09:57
 Operator : SY/MD
 Sample : P1856-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.896	1197	1199	1201	rBV	499	271	0.02%	0.002%
38	4.953	1202	1217	1253	rBV2	564942	1511117	100.00%	13.393%
39	5.461	1373	1375	1380	rVB3	546	337	0.02%	0.003%
40	5.532	1386	1397	1431	rBV	406237	850324	56.27%	7.536%
41	5.834	1480	1491	1511	rBV3	12499	29638	1.96%	0.263%
42	5.985	1525	1538	1574	rBV	332388	690116	45.67%	6.116%
43	6.323	1639	1643	1647	rBV5	675	608	0.04%	0.005%
44	6.442	1677	1680	1684	rBV2	702	437	0.03%	0.004%
45	6.477	1684	1691	1692	rBV3	547	461	0.03%	0.004%
46	6.500	1697	1698	1701	rVB2	406	141	0.01%	0.001%
47	6.548	1710	1713	1718	rBV3	487	411	0.03%	0.004%
48	6.635	1738	1740	1745	rBV2	300	255	0.02%	0.002%
49	6.728	1763	1769	1771	rBV2	364	370	0.02%	0.003%
50	6.783	1783	1786	1789	rVB3	329	173	0.01%	0.002%
51	6.799	1789	1791	1793	rBV2	349	137	0.01%	0.001%
52	6.844	1803	1805	1810	rBV2	332	288	0.02%	0.003%
53	6.911	1816	1826	1859	rVV	166949	322393	21.33%	2.857%
54	7.182	1908	1910	1914	rBV5	457	250	0.02%	0.002%
55	7.243	1918	1929	1956	rBV	672843	1190090	78.76%	10.547%
56	7.551	2016	2025	2050	rBV	112394	212612	14.07%	1.884%
57	7.863	2119	2122	2126	rBV3	380	314	0.02%	0.003%
58	7.899	2130	2133	2134	rBV	288	162	0.01%	0.001%
59	7.934	2142	2144	2147	rBV2	353	173	0.01%	0.002%
60	7.979	2155	2158	2162	rVB3	672	457	0.03%	0.004%
61	8.027	2164	2173	2218	rBV2	259872	620121	41.04%	5.496%
62	8.410	2290	2292	2294	rBV2	579	249	0.02%	0.002%
63	8.609	2347	2354	2356	rBV4	483	475	0.03%	0.004%
64	8.738	2391	2394	2396	rBV2	402	253	0.02%	0.002%
65	8.783	2397	2408	2437	rBV	642358	1071303	70.89%	9.495%
66	9.066	2494	2496	2501	rVB3	664	531	0.04%	0.005%
67	9.153	2519	2523	2525	rBV4	519	376	0.02%	0.003%
68	9.207	2539	2540	2542	rBV	300	132	0.01%	0.001%
69	9.262	2555	2557	2561	rBV3	477	343	0.02%	0.003%
70	9.317	2571	2574	2580	rBV5	397	382	0.03%	0.003%
71	9.522	2635	2638	2640	rBV	190	115	0.01%	0.001%
72	9.609	2663	2665	2667	rVV	279	152	0.01%	0.001%
73	9.645	2673	2676	2677	rBV	314	151	0.01%	0.001%
74	9.799	2721	2724	2727	rBV2	430	272	0.02%	0.002%
75	9.870	2744	2746	2750	rBV	506	362	0.02%	0.003%
76	9.944	2767	2769	2775	rVB3	477	421	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034897.D
 Acq On : 29 Mar 2024 09:57
 Operator : SY/MD
 Sample : P1856-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.011	2786	2790	2795	rVB3	546	430	0.03%	0.004%
78	10.050	2796	2802	2806	rBV3	673	678	0.04%	0.006%
79	10.149	2822	2833	2860	rBV	440586	688242	45.55%	6.100%
80	10.365	2896	2900	2905	rBV3	608	632	0.04%	0.006%
81	10.387	2905	2907	2911	rVB2	318	141	0.01%	0.001%
82	10.487	2935	2938	2941	rVB3	484	264	0.02%	0.002%
83	10.571	2963	2964	2967	rVB	461	151	0.01%	0.001%
84	10.738	3013	3016	3017	rBV	344	209	0.01%	0.002%
85	10.789	3029	3032	3035	rVB	582	351	0.02%	0.003%
86	10.808	3035	3038	3042	rBV2	453	463	0.03%	0.004%
87	10.863	3050	3055	3056	rBV2	424	350	0.02%	0.003%
88	11.136	3133	3140	3144	rBV5	1171	1361	0.09%	0.012%
89	11.185	3144	3155	3185	rVV	658749	1020945	67.56%	9.048%
90	11.416	3225	3227	3231	rBV2	370	261	0.02%	0.002%
91	11.558	3259	3271	3298	rBV	658229	1063442	70.37%	9.425%
92	11.818	3350	3352	3354	rBV3	477	228	0.02%	0.002%
93	12.149	3453	3455	3456	rBV2	421	170	0.01%	0.002%
94	12.529	3569	3573	3575	rBV	432	294	0.02%	0.003%
95	12.648	3607	3610	3614	rBV3	607	550	0.04%	0.005%
96	12.860	3674	3676	3678	rBV	366	165	0.01%	0.001%
97	13.207	3777	3784	3792	rBV3	2939	4328	0.29%	0.038%
98	13.361	3828	3832	3835	rBV2	374	384	0.03%	0.003%
99	13.445	3852	3858	3871	rBV3	6582	11922	0.79%	0.106%
100	14.014	4033	4035	4039	rBV3	519	434	0.03%	0.004%




Sum of corrected areas: 11283166

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034897.D
Acq On : 29 Mar 2024 09:57
Operator : SY/MD
Sample : P1856-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

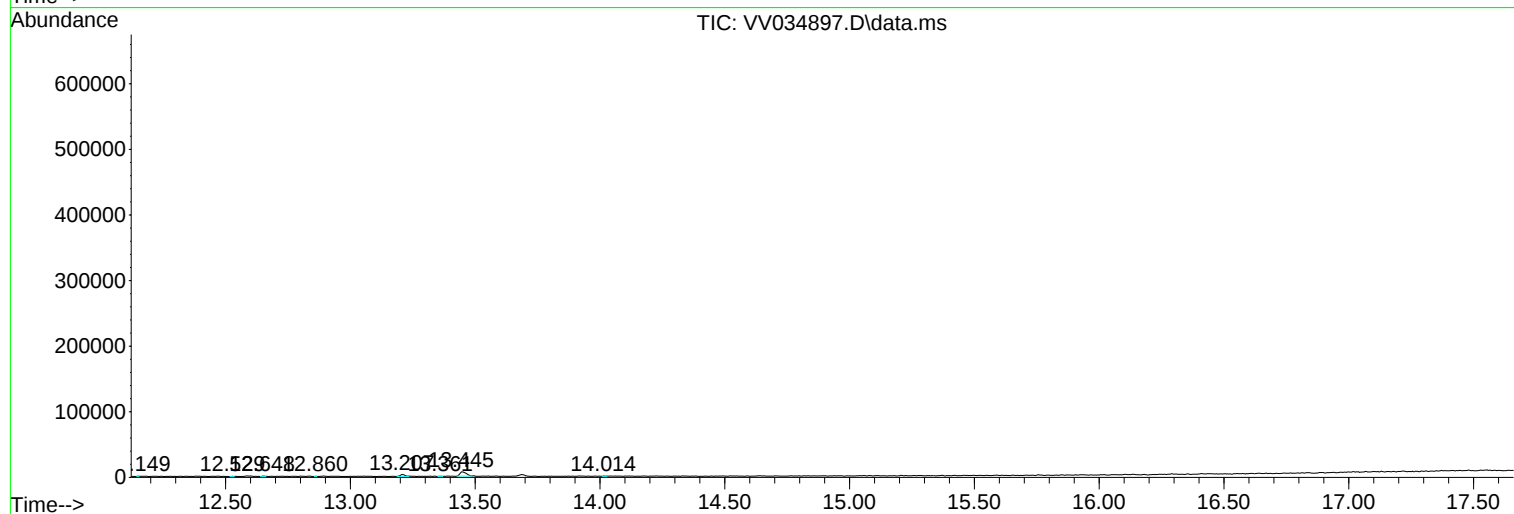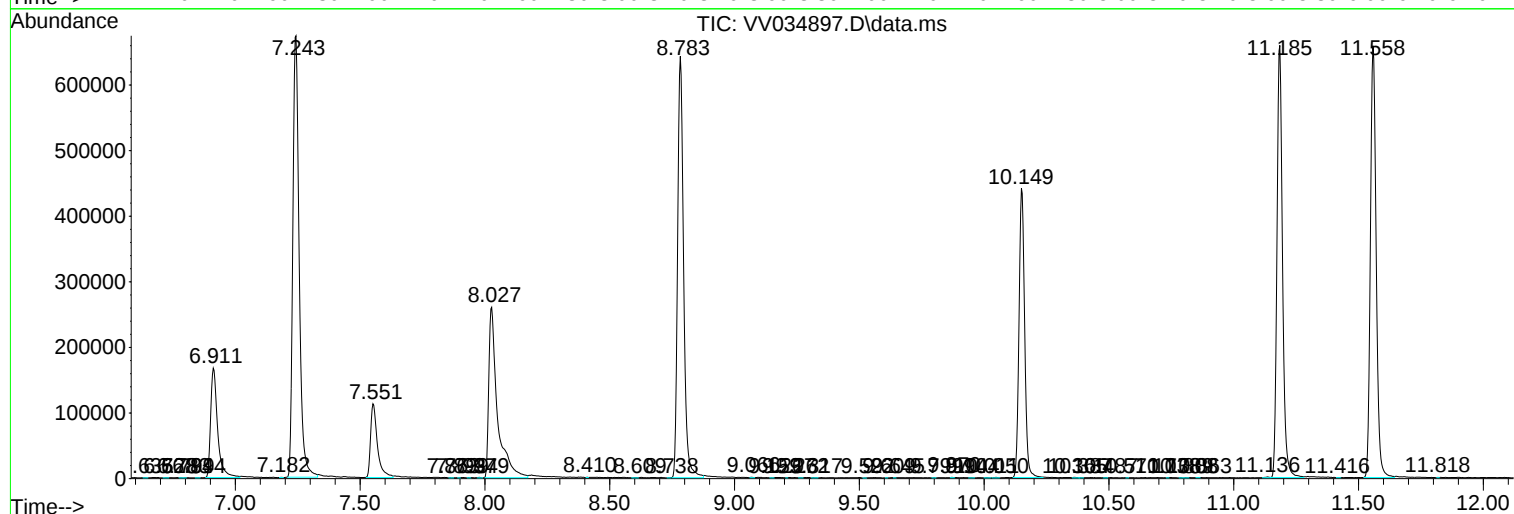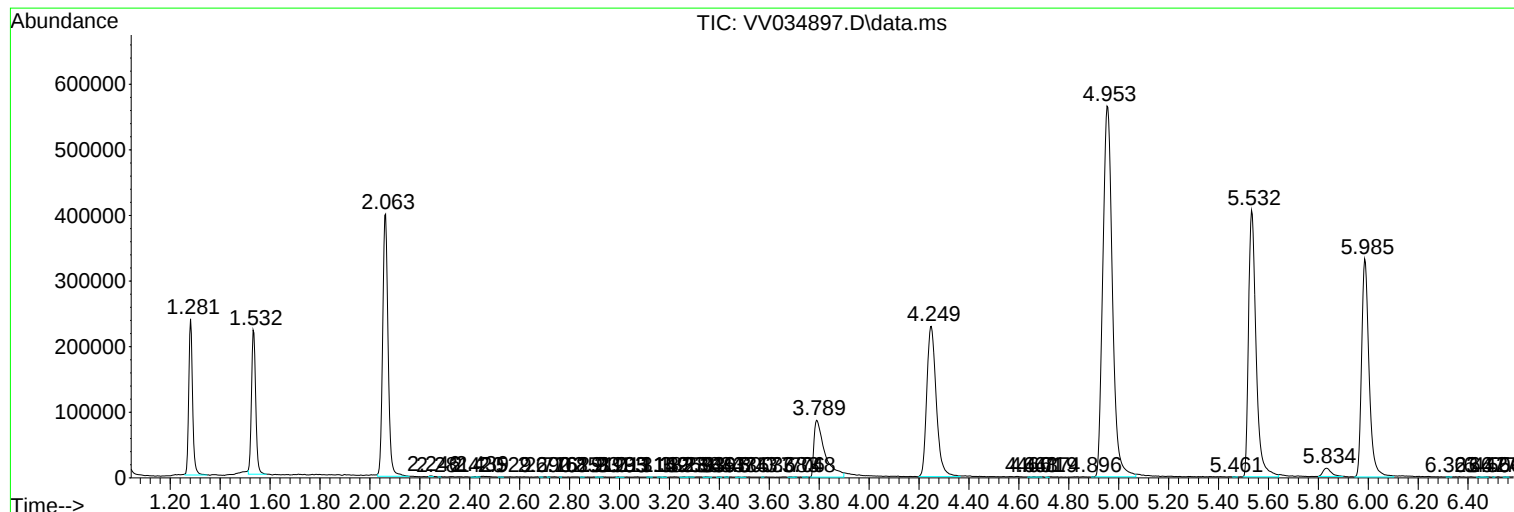

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034897.D
Acq On : 29 Mar 2024 09:57
Operator : SY/MD
Sample : P1856-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034897.D
Acq On : 29 Mar 2024 09:57
Operator : SY/MD
Sample : P1856-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------