

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034898.D
 Acq On : 29 Mar 2024 10:21
 Operator : SY/MD
 Sample : P1822-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	228744	241094	16.18%	2.174%
2	1.536	147	154	170	rVB	209847	249791	16.76%	2.252%
3	2.063	308	318	334	rBV	388216	567196	38.07%	5.113%
4	2.355	406	409	414	rBV3	543	387	0.03%	0.003%
5	2.413	425	427	429	rBV2	404	251	0.02%	0.002%
6	2.523	458	461	463	rBV	499	432	0.03%	0.004%
7	2.587	478	481	486	rVB3	572	565	0.04%	0.005%
8	2.648	497	500	501	rBV	393	221	0.01%	0.002%
9	2.728	521	525	529	rBV2	250	242	0.02%	0.002%
10	2.818	550	553	554	rBV	257	174	0.01%	0.002%
11	2.880	571	572	574	rBV	427	168	0.01%	0.002%
12	2.902	576	579	581	rVV2	520	252	0.02%	0.002%
13	2.931	586	588	590	rBV	274	151	0.01%	0.001%
14	3.031	616	619	626	rVB2	475	335	0.02%	0.003%
15	3.063	626	629	630	rBV	332	182	0.01%	0.002%
16	3.098	638	640	645	rVB3	390	248	0.02%	0.002%
17	3.134	650	651	654	rBV	268	137	0.01%	0.001%
18	3.172	659	663	665	rBV2	314	259	0.02%	0.002%
19	3.208	670	674	675	rBV2	224	161	0.01%	0.001%
20	3.259	687	690	692	rBV2	187	147	0.01%	0.001%
21	3.310	698	706	707	rBV2	548	413	0.03%	0.004%
22	3.339	711	715	718	rVB3	368	336	0.02%	0.003%
23	3.433	739	744	749	rBV3	360	382	0.03%	0.003%
24	3.494	759	763	766	rBV2	381	287	0.02%	0.003%
25	3.548	777	780	784	rBV2	288	204	0.01%	0.002%
26	3.590	791	793	794	rBV	318	139	0.01%	0.001%
27	3.600	794	796	800	rVB2	308	206	0.01%	0.002%
28	3.709	828	830	833	rBV	285	143	0.01%	0.001%
29	3.790	847	855	897	rBV	93584	283179	19.01%	2.553%
30	4.249	983	998	1026	rBV	228374	588214	39.48%	5.303%
31	4.661	1123	1126	1128	rBV2	355	195	0.01%	0.002%
32	4.677	1128	1131	1133	rBV2	401	240	0.02%	0.002%
33	4.793	1164	1167	1170	rBV2	319	196	0.01%	0.002%
34	4.815	1172	1174	1176	rVB3	370	142	0.01%	0.001%
35	4.860	1185	1188	1191	rVB3	313	193	0.01%	0.002%
36	4.957	1202	1218	1246	rBV2	564985	1489991	100.00%	13.433%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034898.D
 Acq On : 29 Mar 2024 10:21
 Operator : SY/MD
 Sample : P1822-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.433	1363	1366	1369	rBV4	518	347	0.02%	0.003%
38	5.532	1386	1397	1431	rBV	397003	835407	56.07%	7.532%
39	5.831	1480	1490	1506	rBV4	13301	30916	2.07%	0.279%
40	5.986	1526	1538	1565	rBV	322096	674344	45.26%	6.079%
41	6.336	1645	1647	1650	rBV2	503	246	0.02%	0.002%
42	6.429	1672	1676	1678	rBV	275	232	0.02%	0.002%
43	6.481	1689	1692	1693	rBV2	306	177	0.01%	0.002%
44	6.548	1710	1713	1715	rBV2	314	214	0.01%	0.002%
45	6.561	1715	1717	1719	rVV	415	190	0.01%	0.002%
46	6.587	1723	1725	1729	rVB2	352	242	0.02%	0.002%
47	6.635	1737	1740	1745	rVB3	434	323	0.02%	0.003%
48	6.677	1749	1753	1754	rBV	462	275	0.02%	0.002%
49	6.735	1769	1771	1773	rVB	327	150	0.01%	0.001%
50	6.789	1786	1788	1795	rVB3	423	341	0.02%	0.003%
51	6.912	1816	1826	1854	rBV	164837	321695	21.59%	2.900%
52	7.243	1918	1929	1952	rBV	655861	1159467	77.82%	10.453%
53	7.551	2016	2025	2056	rBV	113886	215201	14.44%	1.940%
54	7.776	2093	2095	2098	rVB2	682	225	0.02%	0.002%
55	7.847	2115	2117	2118	rBV	378	153	0.01%	0.001%
56	7.908	2134	2136	2143	rVB3	503	315	0.02%	0.003%
57	7.937	2143	2145	2147	rBV	391	203	0.01%	0.002%
58	8.027	2163	2173	2208	rBV2	271966	637965	42.82%	5.751%
59	8.683	2375	2377	2381	rBV3	540	402	0.03%	0.004%
60	8.702	2381	2383	2386	rVB2	844	521	0.03%	0.005%
61	8.722	2386	2389	2390	rBV	538	318	0.02%	0.003%
62	8.783	2397	2408	2445	rBV	633035	1047531	70.30%	9.444%
63	9.137	2515	2518	2521	rBV2	542	444	0.03%	0.004%
64	9.191	2533	2535	2539	rBV	390	300	0.02%	0.003%
65	9.262	2555	2557	2560	rBV	313	164	0.01%	0.001%
66	9.468	2618	2621	2625	rVB2	386	267	0.02%	0.002%
67	9.538	2638	2643	2646	rVB3	432	298	0.02%	0.003%
68	9.555	2646	2648	2654	rBV2	409	308	0.02%	0.003%
69	9.583	2654	2657	2659	rBV	376	188	0.01%	0.002%
70	9.596	2659	2661	2662	rBV	460	139	0.01%	0.001%
71	9.635	2670	2673	2677	rBV	369	282	0.02%	0.003%
72	9.664	2678	2682	2683	rBV2	392	248	0.02%	0.002%
73	9.712	2695	2697	2701	rVB2	448	218	0.01%	0.002%
74	9.818	2728	2730	2734	rVB2	254	159	0.01%	0.001%
75	9.889	2750	2752	2754	rBV	255	143	0.01%	0.001%
76	9.992	2781	2784	2786	rBV	279	147	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034898.D
 Acq On : 29 Mar 2024 10:21
 Operator : SY/MD
 Sample : P1822-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs : 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2821	2833	2860	rBV	450494	705913	47.38%	6.364%
78	10.410	2912	2914	2916	rBV2	318	138	0.01%	0.001%
79	10.574	2963	2965	2967	rBV	363	175	0.01%	0.002%
80	10.728	3008	3013	3015	rVB2	433	373	0.03%	0.003%
81	10.805	3033	3037	3038	rBV	475	264	0.02%	0.002%
82	10.944	3078	3080	3085	rBV2	302	237	0.02%	0.002%
83	11.008	3095	3100	3102	rBV3	427	428	0.03%	0.004%
84	11.127	3131	3137	3143	rBV5	1171	1439	0.10%	0.013%
85	11.185	3143	3155	3175	rBV	613159	978796	65.69%	8.824%
86	11.558	3257	3271	3291	rBV	652233	1035711	69.51%	9.337%
87	11.789	3340	3343	3344	rBV	484	292	0.02%	0.003%
88	12.062	3423	3428	3431	rBV3	422	351	0.02%	0.003%
89	12.262	3488	3490	3493	rBV2	331	184	0.01%	0.002%
90	12.474	3553	3556	3559	rBV2	384	247	0.02%	0.002%
91	12.593	3589	3593	3599	rBV4	1208	1227	0.08%	0.011%
92	12.638	3605	3607	3608	rBV2	309	141	0.01%	0.001%
93	12.673	3617	3618	3621	rBV	288	212	0.01%	0.002%
94	12.757	3641	3644	3649	rBV2	699	588	0.04%	0.005%
95	12.863	3675	3677	3679	rVB	461	188	0.01%	0.002%
96	12.882	3679	3683	3685	rBV	288	220	0.01%	0.002%
97	13.403	3843	3845	3846	rBV	427	143	0.01%	0.001%
98	13.452	3854	3860	3871	rVB3	3967	6245	0.42%	0.056%
99	13.677	3927	3930	3931	rBV2	1054	558	0.04%	0.005%
100	13.982	4021	4025	4027	rBV2	694	542	0.04%	0.005%




Sum of corrected areas: 11092170

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034898.D
Acq On : 29 Mar 2024 10:21
Operator : SY/MD
Sample : P1822-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

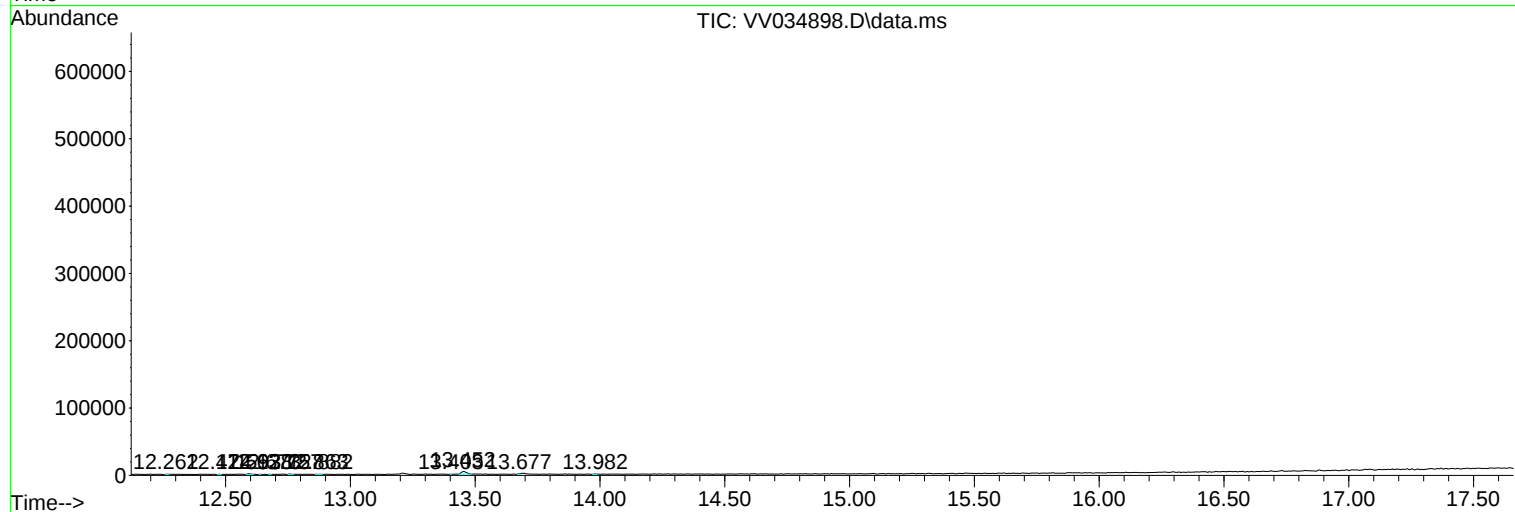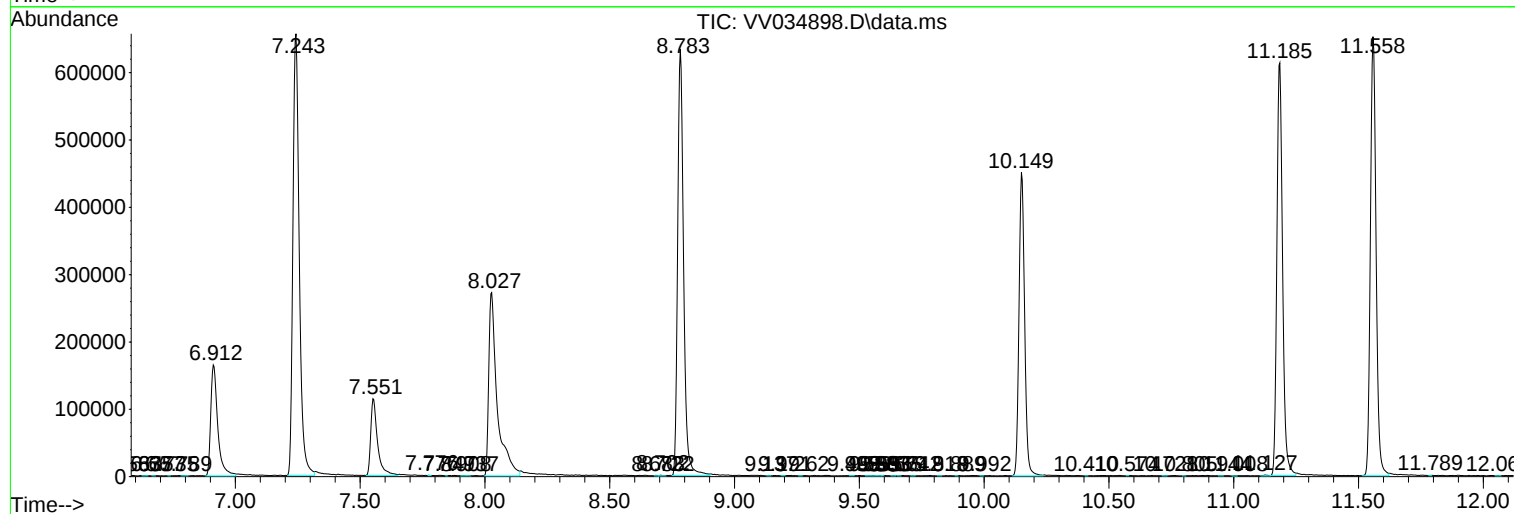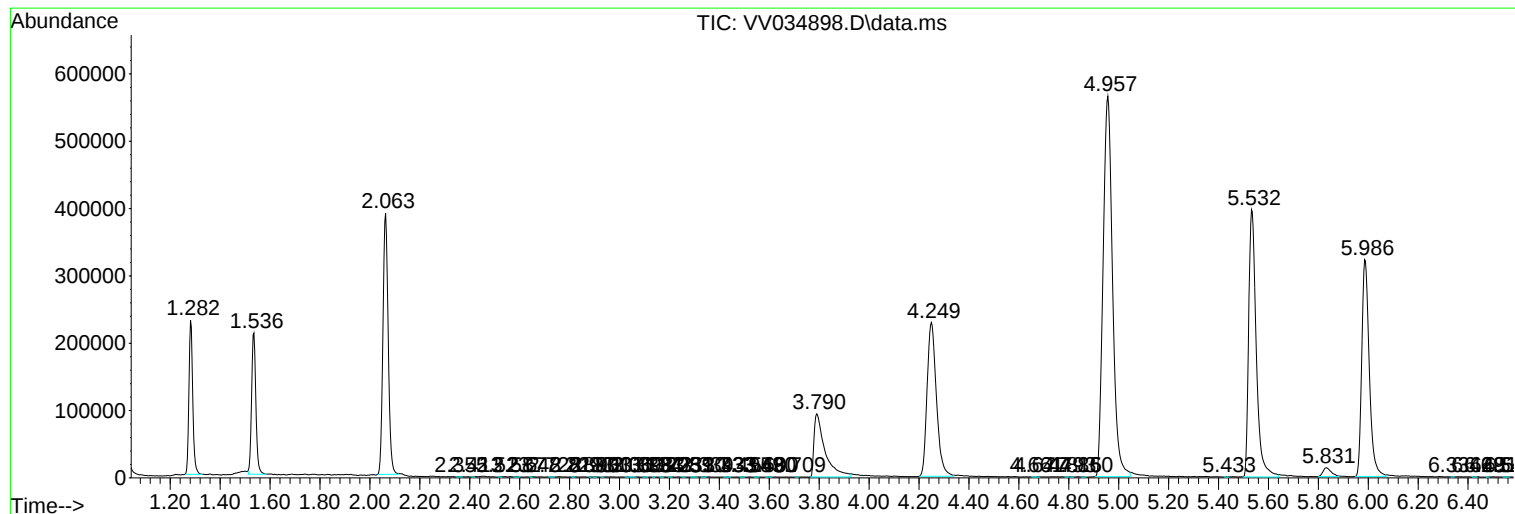

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034898.D
Acq On : 29 Mar 2024 10:21
Operator : SY/MD
Sample : P1822-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034898.D
Acq On : 29 Mar 2024 10:21
Operator : SY/MD
Sample : P1822-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------