

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034899.D
 Acq On : 29 Mar 2024 10:45
 Operator : SY/MD
 Sample : P1886-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0790

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	91	rVB	226976	237504	16.83%	2.450%
2	1.532	146	153	168	rVB	195296	229488	16.26%	2.367%
3	2.060	308	317	330	rBV	376382	543633	38.51%	5.608%
4	2.404	422	424	426	rVB2	411	144	0.01%	0.001%
5	2.446	431	437	438	rBV4	855	781	0.06%	0.008%
6	2.667	501	506	507	rBV3	337	289	0.02%	0.003%
7	2.754	529	533	537	rBV2	364	343	0.02%	0.004%
8	2.863	563	567	569	rBV3	253	175	0.01%	0.002%
9	2.921	583	585	588	rBV	267	146	0.01%	0.002%
10	3.037	616	621	623	rBV2	334	247	0.02%	0.003%
11	3.108	640	643	648	rVB2	330	232	0.02%	0.002%
12	3.156	654	658	661	rVB3	355	284	0.02%	0.003%
13	3.182	661	666	670	rBV2	270	325	0.02%	0.003%
14	3.214	673	676	679	rVV2	309	229	0.02%	0.002%
15	3.246	683	686	688	rBV2	314	240	0.02%	0.002%
16	3.278	690	696	700	rBV4	410	361	0.03%	0.004%
17	3.400	730	734	735	rBV2	391	223	0.02%	0.002%
18	3.436	741	745	747	rBV	218	147	0.01%	0.002%
19	3.497	762	764	769	rBV	205	169	0.01%	0.002%
20	3.683	820	822	826	rVB2	515	259	0.02%	0.003%
21	3.706	826	829	832	rBV2	253	148	0.01%	0.002%
22	3.789	847	855	889	rBV	79278	236306	16.74%	2.438%
23	4.249	979	998	1032	rBV	223550	630154	44.64%	6.500%
24	4.732	1143	1148	1150	rBV3	477	410	0.03%	0.004%
25	4.789	1163	1166	1173	rBV2	453	483	0.03%	0.005%
26	4.854	1183	1186	1191	rVB3	502	512	0.04%	0.005%
27	4.883	1191	1195	1196	rBV	313	230	0.02%	0.002%
28	4.957	1202	1218	1260	rBV2	526834	1411515	100.00%	14.560%
29	5.400	1352	1356	1360	rBV3	662	547	0.04%	0.006%
30	5.445	1368	1370	1372	rBV2	434	175	0.01%	0.002%
31	5.535	1387	1398	1436	rBV	260738	561798	39.80%	5.795%
32	5.834	1480	1491	1505	rBV4	14476	32791	2.32%	0.338%
33	5.986	1526	1538	1569	rBV	308070	639627	45.31%	6.598%
34	6.278	1628	1629	1632	rBV2	357	180	0.01%	0.002%
35	6.378	1657	1660	1661	rBV2	431	186	0.01%	0.002%
36	6.445	1672	1681	1694	rVB4	5556	11073	0.78%	0.114%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034899.D
 Acq On : 29 Mar 2024 10:45
 Operator : SY/MD
 Sample : P1886-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0790

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.590	1722	1726	1728	rBV2	525	277	0.02%	0.003%
38	6.606	1728	1731	1735	rBV3	258	265	0.02%	0.003%
39	6.648	1741	1744	1747	rBV	378	266	0.02%	0.003%
40	6.674	1750	1752	1755	rVV3	570	384	0.03%	0.004%

41	6.741	1768	1773	1776	rVB4	370	246	0.02%	0.003%
42	6.764	1776	1780	1782	rBV2	421	250	0.02%	0.003%
43	6.796	1787	1790	1794	rVB	206	177	0.01%	0.002%
44	6.847	1803	1806	1808	rBV2	279	150	0.01%	0.002%
45	6.912	1815	1826	1864	rBV	152024	301741	21.38%	3.112%

46	7.243	1918	1929	1953	rBV	625219	1103499	78.18%	11.383%
47	7.551	2016	2025	2054	rBV	101879	198016	14.03%	2.043%
48	7.857	2117	2120	2123	rVB	512	354	0.03%	0.004%
49	7.879	2125	2127	2132	rVB2	477	253	0.02%	0.003%
50	7.902	2132	2134	2139	rBV2	495	463	0.03%	0.005%

51	8.027	2164	2173	2214	rBV2	235643	558535	39.57%	5.761%
52	8.596	2349	2350	2353	rBV3	569	291	0.02%	0.003%
53	8.696	2379	2381	2383	rBV	476	270	0.02%	0.003%
54	8.783	2398	2408	2433	rBV	422404	708070	50.16%	7.304%
55	9.014	2477	2480	2483	rBV3	956	622	0.04%	0.006%

56	9.098	2504	2506	2507	rBV	527	192	0.01%	0.002%
57	9.149	2519	2522	2524	rBV2	567	311	0.02%	0.003%
58	9.198	2533	2537	2542	rBV3	652	549	0.04%	0.006%
59	9.307	2569	2571	2576	rBV	294	199	0.01%	0.002%
60	9.445	2611	2614	2616	rBV	276	185	0.01%	0.002%

61	9.481	2620	2625	2627	rBV2	572	527	0.04%	0.005%
62	9.519	2631	2637	2640	rBV4	1743	1848	0.13%	0.019%
63	9.583	2655	2657	2659	rVB	408	141	0.01%	0.001%
64	9.680	2685	2687	2690	rVV2	374	201	0.01%	0.002%
65	9.699	2690	2693	2696	rVB2	400	204	0.01%	0.002%

66	9.744	2703	2707	2709	rBV	439	324	0.02%	0.003%
67	9.831	2732	2734	2735	rBV	491	156	0.01%	0.002%
68	9.870	2742	2746	2748	rBV2	687	533	0.04%	0.005%
69	9.905	2751	2757	2760	rVV2	331	378	0.03%	0.004%
70	9.924	2760	2763	2765	rBV	326	210	0.01%	0.002%

71	9.969	2772	2777	2780	rBV2	449	416	0.03%	0.004%
72	10.091	2814	2815	2818	rBV	271	147	0.01%	0.002%
73	10.108	2818	2820	2822	rBV2	350	157	0.01%	0.002%
74	10.149	2822	2833	2860	rBV	396670	633216	44.86%	6.532%
75	10.391	2905	2908	2912	rVB2	664	459	0.03%	0.005%

76	10.445	2923	2925	2927	rBV2	403	174	0.01%	0.002%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034899.D
 Acq On : 29 Mar 2024 10:45
 Operator : SY/MD
 Sample : P1886-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0790

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.474	2930	2934	2936	rBV2	284	256	0.02%	0.003%
78	10.542	2953	2955	2958	rBV2	360	214	0.02%	0.002%
79	10.622	2978	2980	2984	rBV2	353	217	0.02%	0.002%
80	10.718	3005	3010	3013	rBV3	575	563	0.04%	0.006%
81	10.815	3034	3040	3044	rBV	522	616	0.04%	0.006%
82	10.866	3052	3056	3058	rVB3	450	311	0.02%	0.003%
83	10.937	3076	3078	3081	rBV	362	270	0.02%	0.003%
84	11.005	3096	3099	3101	rBV	364	252	0.02%	0.003%
85	11.127	3135	3137	3138	rBV	539	187	0.01%	0.002%
86	11.185	3144	3155	3178	rBV	421496	664473	47.08%	6.854%
87	11.461	3238	3241	3243	rVB2	555	339	0.02%	0.003%
88	11.558	3260	3271	3292	rBV	613708	965380	68.39%	9.958%
89	11.876	3367	3370	3373	rBV3	299	237	0.02%	0.002%
90	12.259	3485	3489	3490	rBV2	498	325	0.02%	0.003%
91	12.316	3505	3507	3508	rBV2	356	145	0.01%	0.001%
92	12.500	3562	3564	3567	rVV2	535	331	0.02%	0.003%
93	12.593	3591	3593	3597	rVB3	692	521	0.04%	0.005%
94	12.728	3632	3635	3638	rBV2	458	323	0.02%	0.003%
95	12.767	3644	3647	3649	rBV2	410	239	0.02%	0.002%
96	12.779	3649	3651	3657	rVV	363	323	0.02%	0.003%
97	12.931	3696	3698	3703	rVB2	591	316	0.02%	0.003%
98	13.214	3780	3786	3789	rBV3	990	1357	0.10%	0.014%
99	13.570	3895	3897	3901	rBV2	459	312	0.02%	0.003%
100	13.744	3946	3951	3957	rBV3	787	1082	0.08%	0.011%




Sum of corrected areas: 9694599

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034899.D
Acq On : 29 Mar 2024 10:45
Operator : SY/MD
Sample : P1886-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0790

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

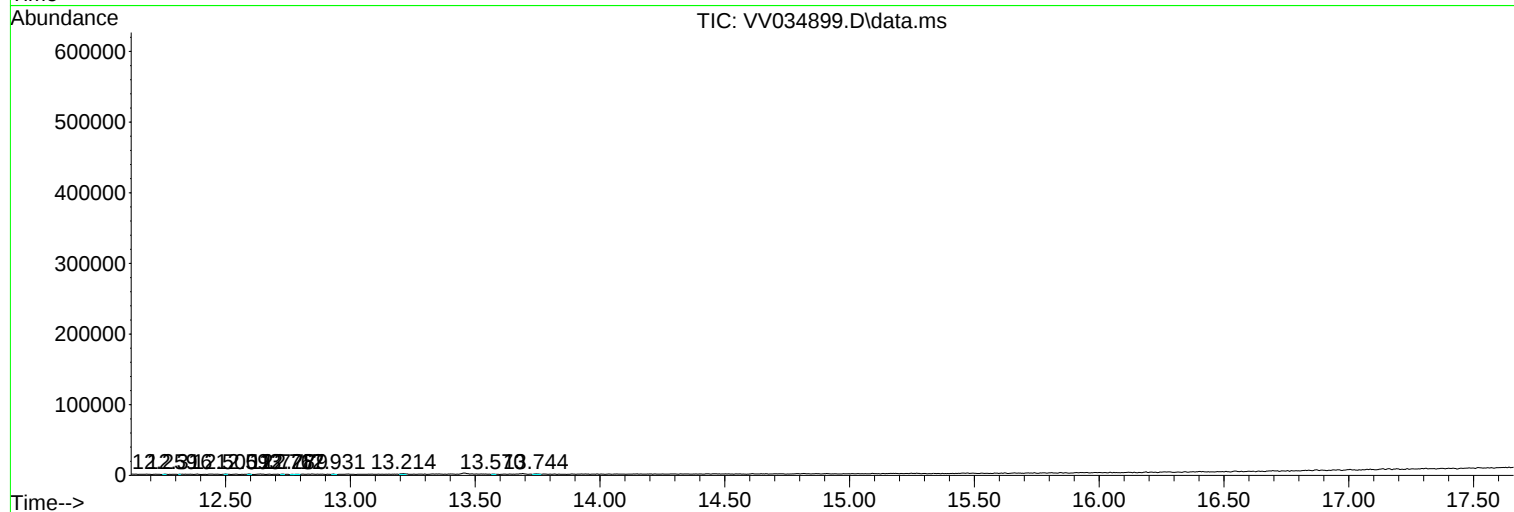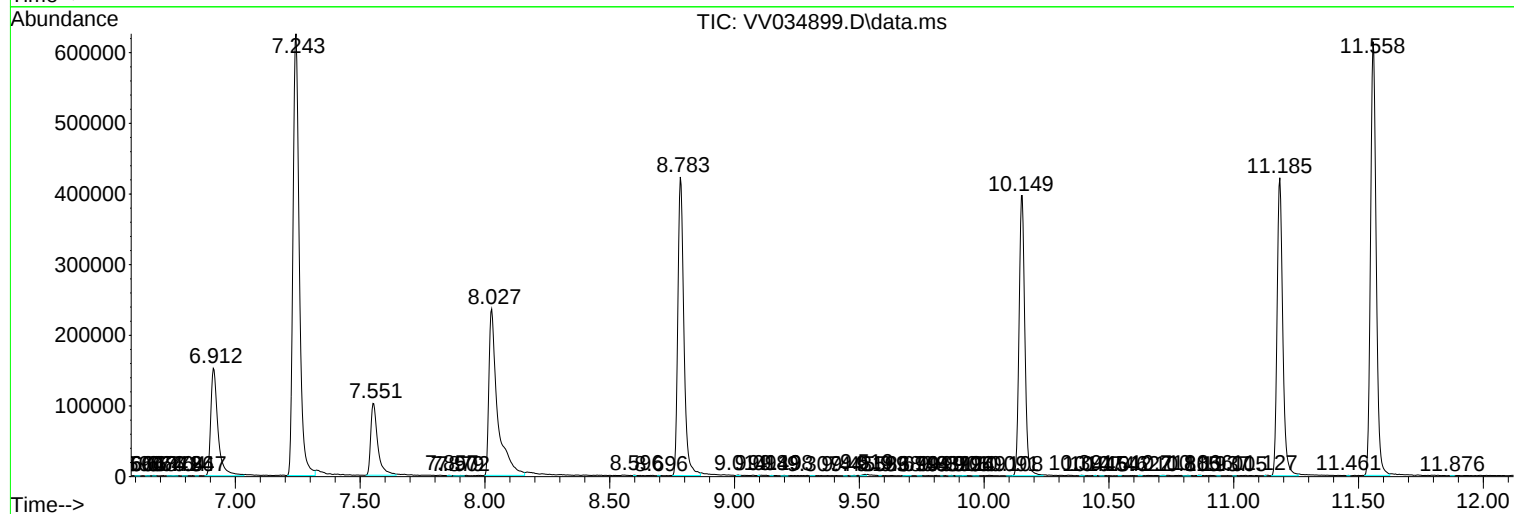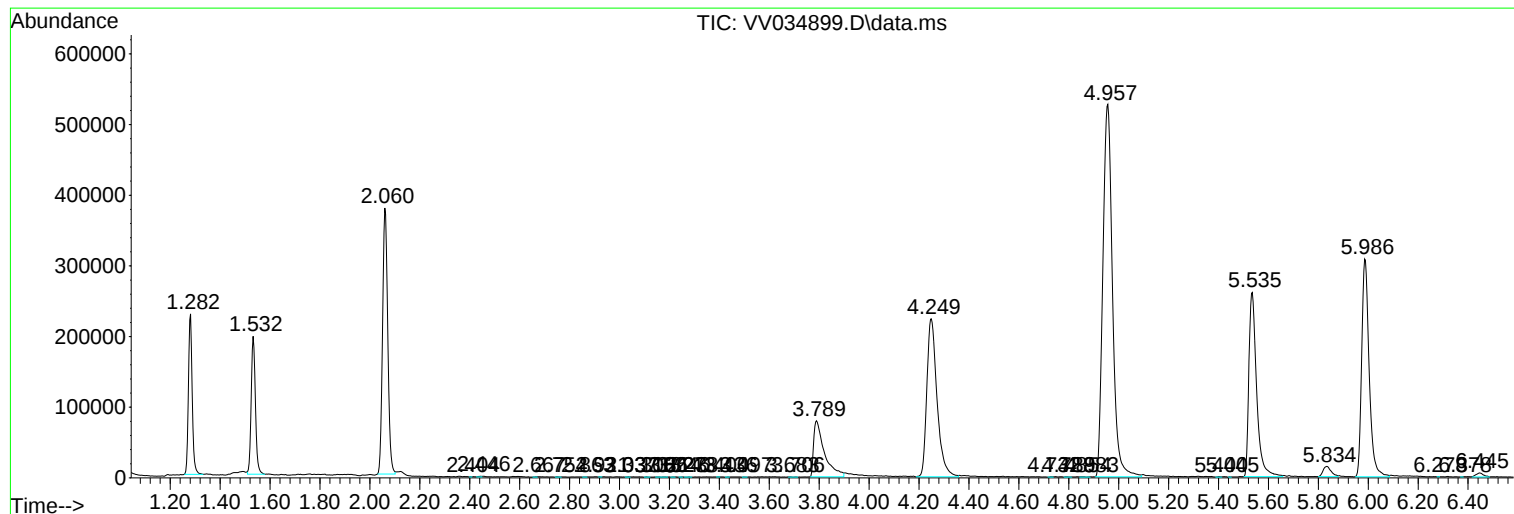

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034899.D
Acq On : 29 Mar 2024 10:45
Operator : SY/MD
Sample : P1886-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0790

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034899.D
Acq On : 29 Mar 2024 10:45
Operator : SY/MD
Sample : P1886-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0790

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------