

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034901.D
 Acq On : 29 Mar 2024 11:32
 Operator : SY/MD
 Sample : P1886-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	42	47	53	rBV	12184	11660	0.91%	0.119%
2	1.282	67	75	91	rVB	204399	222664	17.33%	2.279%
3	1.532	146	153	166	rVB	183046	214018	16.66%	2.190%
4	2.060	308	317	332	rBV	342230	497255	38.70%	5.088%
5	2.307	392	394	397	rBV	632	414	0.03%	0.004%
6	2.449	434	438	442	rBV5	920	934	0.07%	0.010%
7	2.500	451	454	457	rBV3	625	401	0.03%	0.004%
8	2.677	507	509	516	rBV4	468	463	0.04%	0.005%
9	2.728	523	525	529	rBV2	426	229	0.02%	0.002%
10	2.799	544	547	550	rBV2	597	329	0.03%	0.003%
11	2.828	555	556	561	rVB2	389	231	0.02%	0.002%
12	2.857	561	565	569	rBV2	537	620	0.05%	0.006%
13	2.944	590	592	596	rVB2	475	279	0.02%	0.003%
14	3.021	612	616	622	rVB4	593	548	0.04%	0.006%
15	3.072	629	632	636	rBV2	424	337	0.03%	0.003%
16	3.156	655	658	659	rBV2	347	167	0.01%	0.002%
17	3.243	683	685	688	rBV	255	156	0.01%	0.002%
18	3.330	709	712	715	rVV	326	229	0.02%	0.002%
19	3.381	725	728	729	rBV2	270	166	0.01%	0.002%
20	3.462	751	753	755	rBV	311	176	0.01%	0.002%
21	3.548	775	780	783	rBV	233	259	0.02%	0.003%
22	3.580	786	790	791	rBV	435	264	0.02%	0.003%
23	3.712	825	831	833	rBV2	478	457	0.04%	0.005%
24	3.744	839	841	845	rVB2	476	260	0.02%	0.003%
25	3.789	845	855	897	rBV	77648	242943	18.91%	2.486%
26	4.249	984	998	1033	rVB3	203647	591105	46.01%	6.049%
27	4.651	1121	1123	1125	rBV2	375	224	0.02%	0.002%
28	4.863	1187	1189	1191	rBV2	331	152	0.01%	0.002%
29	4.957	1201	1218	1256	rBV2	486401	1284849	100.00%	13.148%
30	5.207	1294	1296	1299	rBV3	733	530	0.04%	0.005%
31	5.259	1310	1312	1317	rVB3	736	347	0.03%	0.004%
32	5.326	1331	1333	1339	rBV5	537	456	0.04%	0.005%
33	5.352	1339	1341	1343	rBV3	607	258	0.02%	0.003%
34	5.426	1361	1364	1368	rBV3	589	419	0.03%	0.004%
35	5.532	1386	1397	1429	rBV	360045	757390	58.95%	7.750%
36	5.834	1481	1491	1516	rVB2	12430	29440	2.29%	0.301%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034901.D
Acq On : 29 Mar 2024 11:32
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

37	5.989	1526	1539	1567	rBV	274773	581494	45.26%	5.950%
38	6.381	1657	1661	1662	rBV2	498	302	0.02%	0.003%
39	6.391	1662	1664	1669	rBV2	528	503	0.04%	0.005%
40	6.442	1674	1680	1696	rVB3	6885	14278	1.11%	0.146%
41	6.548	1709	1713	1716	rBV2	406	320	0.02%	0.003%
42	6.629	1736	1738	1741	rBV	295	190	0.01%	0.002%
43	6.667	1748	1750	1751	rBV3	285	150	0.01%	0.002%
44	6.722	1760	1767	1769	rBV4	448	473	0.04%	0.005%
45	6.741	1769	1773	1775	rBV	384	281	0.02%	0.003%
46	6.815	1792	1796	1797	rBV2	500	292	0.02%	0.003%
47	6.857	1807	1809	1813	rBV2	419	291	0.02%	0.003%
48	6.912	1817	1826	1853	rBV	139030	270912	21.09%	2.772%
49	7.188	1910	1912	1918	rVB4	647	438	0.03%	0.004%
50	7.243	1918	1929	1950	rBV	569484	1006225	78.31%	10.297%
51	7.555	2016	2026	2054	rBV	94568	183033	14.25%	1.873%
52	7.773	2089	2094	2099	rBV4	817	921	0.07%	0.009%
53	7.834	2110	2113	2119	rBV3	614	508	0.04%	0.005%
54	7.870	2119	2124	2125	rBV2	681	642	0.05%	0.007%
55	7.963	2151	2153	2155	rVB2	428	155	0.01%	0.002%
56	7.995	2161	2163	2164	rBV2	446	181	0.01%	0.002%
57	8.027	2164	2173	2215	rBV3	224645	534382	41.59%	5.468%
58	8.407	2287	2291	2293	rBV2	580	481	0.04%	0.005%
59	8.587	2345	2347	2353	rBV4	429	438	0.03%	0.004%
60	8.664	2368	2371	2375	rBV4	588	477	0.04%	0.005%
61	8.696	2379	2381	2387	rBV2	625	541	0.04%	0.006%
62	8.725	2387	2390	2392	rVB	346	152	0.01%	0.002%
63	8.783	2397	2408	2441	rBV	568007	951177	74.03%	9.733%
64	9.079	2499	2500	2501	rBV	434	148	0.01%	0.002%
65	9.201	2529	2538	2543	rBV4	743	914	0.07%	0.009%
66	9.246	2550	2552	2554	rBV	372	216	0.02%	0.002%
67	9.387	2594	2596	2599	rBV2	345	199	0.02%	0.002%
68	9.452	2614	2616	2622	rVB3	483	398	0.03%	0.004%
69	9.477	2622	2624	2626	rBV2	420	181	0.01%	0.002%
70	9.503	2630	2632	2633	rBV	623	303	0.02%	0.003%
71	9.522	2633	2638	2642	rBV6	1263	1520	0.12%	0.016%
72	9.600	2660	2662	2665	rVB3	617	292	0.02%	0.003%
73	9.680	2685	2687	2690	rVV2	225	159	0.01%	0.002%
74	9.722	2696	2700	2701	rBV2	511	376	0.03%	0.004%
75	9.815	2726	2729	2733	rBV2	377	375	0.03%	0.004%
76	9.860	2740	2743	2744	rBV2	441	244	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034901.D
Acq On : 29 Mar 2024 11:32
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs : 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	9.918	2756	2761	2763	rBV2	656	470	0.04%	0.005%
78	10.063	2803	2806	2807	rBV	434	262	0.02%	0.003%
79	10.149	2822	2833	2856	rBV	365364	583006	45.38%	5.966%
80	10.403	2909	2912	2914	rBV2	495	296	0.02%	0.003%
81	10.522	2947	2949	2950	rBV2	436	189	0.01%	0.002%
82	10.715	3005	3009	3011	rBV2	652	485	0.04%	0.005%
83	10.747	3015	3019	3022	rBV2	253	197	0.02%	0.002%
84	10.863	3053	3055	3059	rBV3	547	218	0.02%	0.002%
85	10.931	3073	3076	3079	rBV2	360	251	0.02%	0.003%
86	10.982	3089	3092	3094	rBV2	477	332	0.03%	0.003%
87	11.046	3109	3112	3113	rBV2	590	312	0.02%	0.003%
88	11.185	3144	3155	3183	rBV	555876	882979	68.72%	9.035%
89	11.426	3228	3230	3235	rBV	411	284	0.02%	0.003%
90	11.458	3235	3240	3243	rBV2	558	414	0.03%	0.004%
91	11.558	3259	3271	3294	rBV	557350	883551	68.77%	9.041%
92	11.921	3382	3384	3387	rBV3	372	232	0.02%	0.002%
93	12.178	3461	3464	3469	rBV3	845	816	0.06%	0.008%
94	12.403	3531	3534	3538	rVB3	706	434	0.03%	0.004%
95	12.490	3557	3561	3566	rVB4	724	621	0.05%	0.006%
96	12.918	3692	3694	3698	rBV	519	326	0.03%	0.003%
97	12.979	3710	3713	3715	rBV2	486	323	0.03%	0.003%
98	13.027	3726	3728	3733	rBV3	487	279	0.02%	0.003%
99	13.120	3755	3757	3762	rBV3	578	497	0.04%	0.005%
100	13.651	3917	3922	3924	rBV3	474	414	0.03%	0.004%




Sum of corrected areas: 9772379

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034901.D
Acq On : 29 Mar 2024 11:32
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

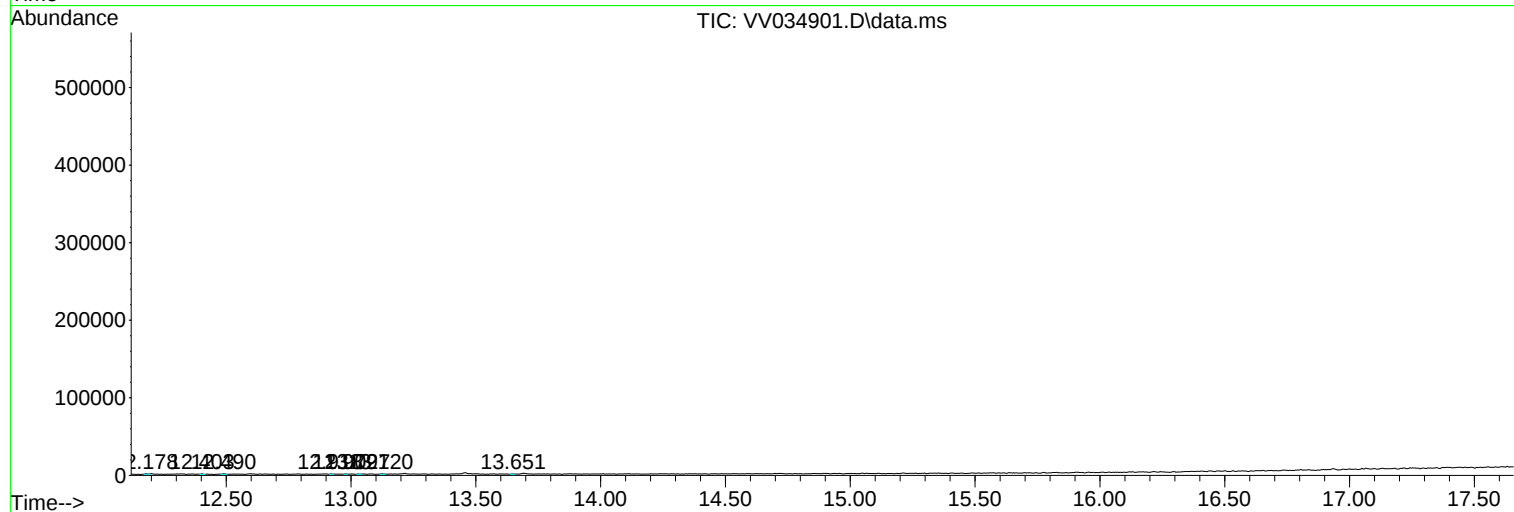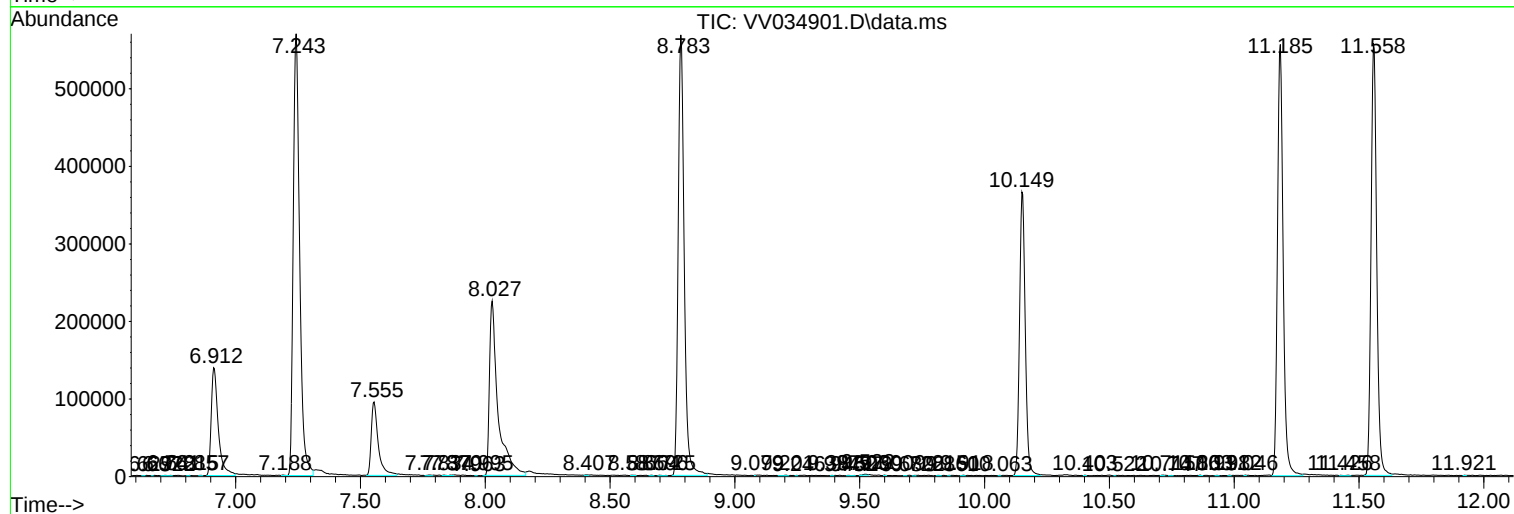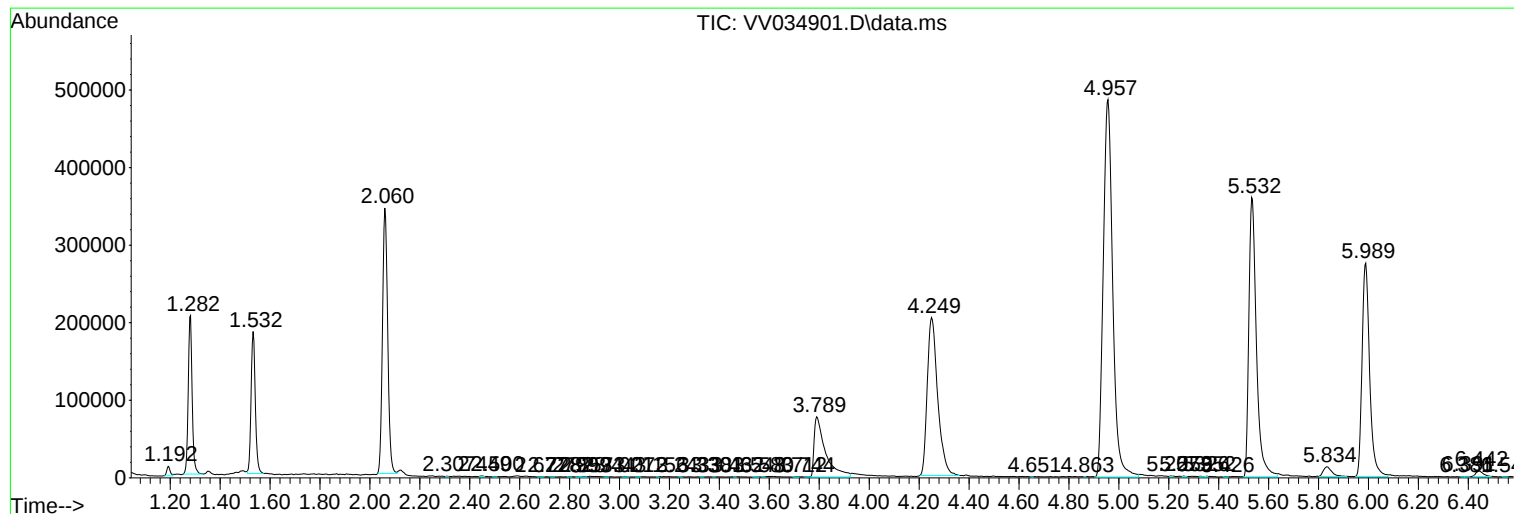

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034901.D
Acq On : 29 Mar 2024 11:32
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034901.D
Acq On : 29 Mar 2024 11:32
Operator : SY/MD
Sample : P1886-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------