

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034903.D
 Acq On : 29 Mar 2024 12:20
 Operator : SY/MD
 Sample : P1886-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	90	rVB	240710	255046	16.88%	2.251%
2	1.532	146	153	165	rVB	221353	255246	16.89%	2.252%
3	2.059	307	317	331	rBV	407344	591271	39.13%	5.217%
4	2.359	405	410	411	rBV4	545	492	0.03%	0.004%
5	2.494	450	452	454	rBV	394	185	0.01%	0.002%
6	2.725	521	524	526	rBV	386	229	0.02%	0.002%
7	2.805	546	549	552	rBV2	284	185	0.01%	0.002%
8	2.825	552	555	557	rBV	212	166	0.01%	0.001%
9	2.854	560	564	566	rBV2	399	261	0.02%	0.002%
10	2.876	568	571	572	rBV2	326	202	0.01%	0.002%
11	2.963	595	598	601	rBV2	447	363	0.02%	0.003%
12	3.140	650	653	655	rVB	217	122	0.01%	0.001%
13	3.153	655	657	658	rBV	255	111	0.01%	0.001%
14	3.195	665	670	674	rBV3	465	348	0.02%	0.003%
15	3.256	686	689	692	rBV	238	188	0.01%	0.002%
16	3.288	696	699	701	rBV2	243	140	0.01%	0.001%
17	3.304	701	704	705	rBV	227	133	0.01%	0.001%
18	3.333	710	713	718	rVV3	418	345	0.02%	0.003%
19	3.358	719	721	725	rVB2	340	241	0.02%	0.002%
20	3.400	733	734	738	rVB	410	120	0.01%	0.001%
21	3.423	739	741	744	rVB2	270	113	0.01%	0.001%
22	3.442	744	747	749	rBV2	242	170	0.01%	0.002%
23	3.487	759	761	765	rVB2	219	131	0.01%	0.001%
24	3.510	765	768	774	rVB2	327	328	0.02%	0.003%
25	3.542	774	778	779	rBV2	527	315	0.02%	0.003%
26	3.564	782	785	787	rBV2	292	167	0.01%	0.001%
27	3.580	787	790	792	rBV3	698	531	0.04%	0.005%
28	3.738	835	839	841	rBV3	339	223	0.01%	0.002%
29	3.789	846	855	899	rBV	90380	281793	18.65%	2.487%
30	4.249	983	998	1028	rBV	241429	659865	43.67%	5.823%
31	4.796	1165	1168	1169	rBV2	391	227	0.02%	0.002%
32	4.834	1178	1180	1185	rVB3	338	244	0.02%	0.002%
33	4.860	1185	1188	1190	rBV3	540	373	0.02%	0.003%
34	4.956	1202	1218	1251	rBV2	571801	1511125	100.00%	13.334%
35	5.368	1344	1346	1348	rBV2	316	152	0.01%	0.001%
36	5.481	1379	1381	1382	rBV2	459	247	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034903.D
Acq On : 29 Mar 2024 12:20
Operator : SY/MD
Sample : P1886-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

37	5.532	1386	1397	1428	rBV	411087	860039	56.91%	7.589%
38	5.831	1482	1490	1508	rVB4	15475	31867	2.11%	0.281%
39	5.985	1526	1538	1568	rBV	326776	684457	45.29%	6.040%
40	6.320	1639	1642	1645	rBV3	389	307	0.02%	0.003%
41	6.374	1657	1659	1660	rBV	261	118	0.01%	0.001%
42	6.384	1660	1662	1666	rVB3	698	412	0.03%	0.004%
43	6.448	1671	1682	1692	rBV3	5759	12151	0.80%	0.107%
44	6.551	1710	1714	1715	rBV	196	142	0.01%	0.001%
45	6.561	1715	1717	1722	rVB2	502	380	0.03%	0.003%
46	6.603	1726	1730	1732	rBV	567	335	0.02%	0.003%
47	6.638	1738	1741	1742	rBV	456	255	0.02%	0.002%
48	6.648	1742	1744	1746	rVV	338	151	0.01%	0.001%
49	6.677	1751	1753	1757	rVV4	343	300	0.02%	0.003%
50	6.696	1757	1759	1763	rVB2	420	245	0.02%	0.002%
51	6.718	1763	1766	1772	rBV3	383	347	0.02%	0.003%
52	6.767	1777	1781	1782	rBV2	178	106	0.01%	0.001%
53	6.792	1787	1789	1790	rBV2	257	103	0.01%	0.001%
54	6.911	1812	1826	1863	rBV	168861	329983	21.84%	2.912%
55	7.185	1909	1911	1915	rVB3	854	412	0.03%	0.004%
56	7.243	1918	1929	1957	rBV	673368	1200943	79.47%	10.597%
57	7.551	2017	2025	2053	rBV	113578	213015	14.10%	1.880%
58	7.837	2112	2114	2116	rBV	571	198	0.01%	0.002%
59	7.989	2159	2161	2162	rBV	404	195	0.01%	0.002%
60	8.027	2163	2173	2214	rVV2	265829	626957	41.49%	5.532%
61	8.654	2365	2368	2373	rVB3	669	426	0.03%	0.004%
62	8.689	2378	2379	2383	rBV2	345	214	0.01%	0.002%
63	8.783	2397	2408	2439	rBV	648497	1074302	71.09%	9.480%
64	9.017	2479	2481	2483	rVB3	524	223	0.01%	0.002%
65	9.030	2483	2485	2487	rBV2	678	310	0.02%	0.003%
66	9.062	2492	2495	2500	rVB4	698	458	0.03%	0.004%
67	9.175	2528	2530	2531	rBV	471	198	0.01%	0.002%
68	9.365	2588	2589	2592	rBV	369	148	0.01%	0.001%
69	9.458	2615	2618	2620	rBV2	332	230	0.02%	0.002%
70	9.519	2634	2637	2646	rBV5	1162	1804	0.12%	0.016%
71	9.587	2657	2658	2660	rBV	220	114	0.01%	0.001%
72	9.628	2669	2671	2672	rBV	292	122	0.01%	0.001%
73	9.683	2683	2688	2690	rBV	323	281	0.02%	0.002%
74	9.760	2707	2712	2714	rBV	476	325	0.02%	0.003%
75	9.792	2718	2722	2728	rVV2	550	549	0.04%	0.005%
76	9.995	2783	2785	2788	rVB2	388	197	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034903.D
 Acq On : 29 Mar 2024 12:20
 Operator : SY/MD
 Sample : P1886-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.008	2788	2789	2790	rBV2	327	104	0.01%	0.001%
78	10.072	2803	2809	2812	rBV2	439	532	0.04%	0.005%
79	10.149	2821	2833	2861	rBV	427745	685704	45.38%	6.051%
80	10.326	2883	2888	2892	rVB3	1128	1077	0.07%	0.010%
81	10.377	2901	2904	2905	rBV	248	137	0.01%	0.001%
82	10.480	2934	2936	2937	rBV	391	163	0.01%	0.001%
83	10.622	2973	2980	2985	rBV2	633	850	0.06%	0.008%
84	10.664	2991	2993	2997	rVB	452	213	0.01%	0.002%
85	10.715	3002	3009	3012	rBV4	473	613	0.04%	0.005%
86	10.908	3067	3069	3071	rBV2	300	165	0.01%	0.001%
87	10.969	3086	3088	3091	rVB	489	179	0.01%	0.002%
88	10.998	3091	3097	3099	rBV2	505	381	0.03%	0.003%
89	11.011	3099	3101	3104	rBV2	236	138	0.01%	0.001%
90	11.075	3119	3121	3123	rBV2	283	133	0.01%	0.001%
91	11.133	3133	3139	3141	rBV4	893	812	0.05%	0.007%
92	11.185	3144	3155	3178	rBV	637756	991608	65.62%	8.750%
93	11.558	3260	3271	3302	rBV	658355	1042428	68.98%	9.198%
94	11.853	3361	3363	3365	rBV2	495	219	0.01%	0.002%
95	12.033	3418	3419	3421	rBV	304	166	0.01%	0.001%
96	12.583	3588	3590	3595	rBV3	919	877	0.06%	0.008%
97	12.792	3653	3655	3656	rBV	480	144	0.01%	0.001%
98	12.834	3666	3668	3674	rVB2	447	280	0.02%	0.002%
99	13.217	3782	3787	3788	rBV2	756	762	0.05%	0.007%
100	13.959	4016	4018	4019	rBV	669	244	0.02%	0.002%




Sum of corrected areas: 11332646

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034903.D
Acq On : 29 Mar 2024 12:20
Operator : SY/MD
Sample : P1886-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

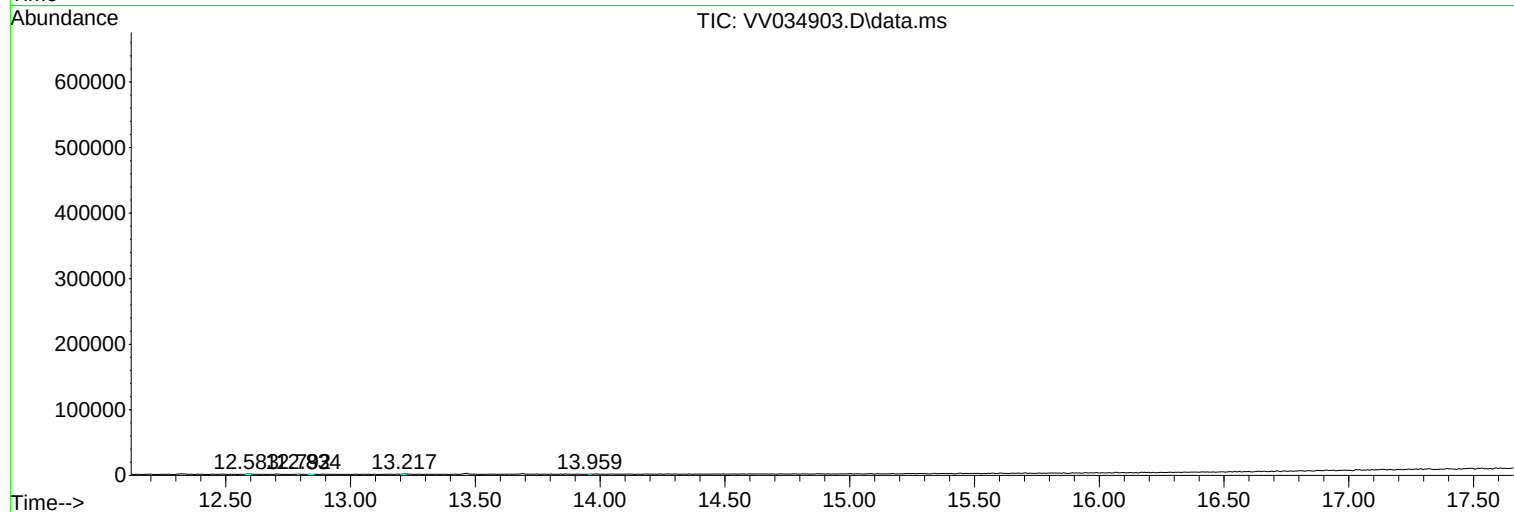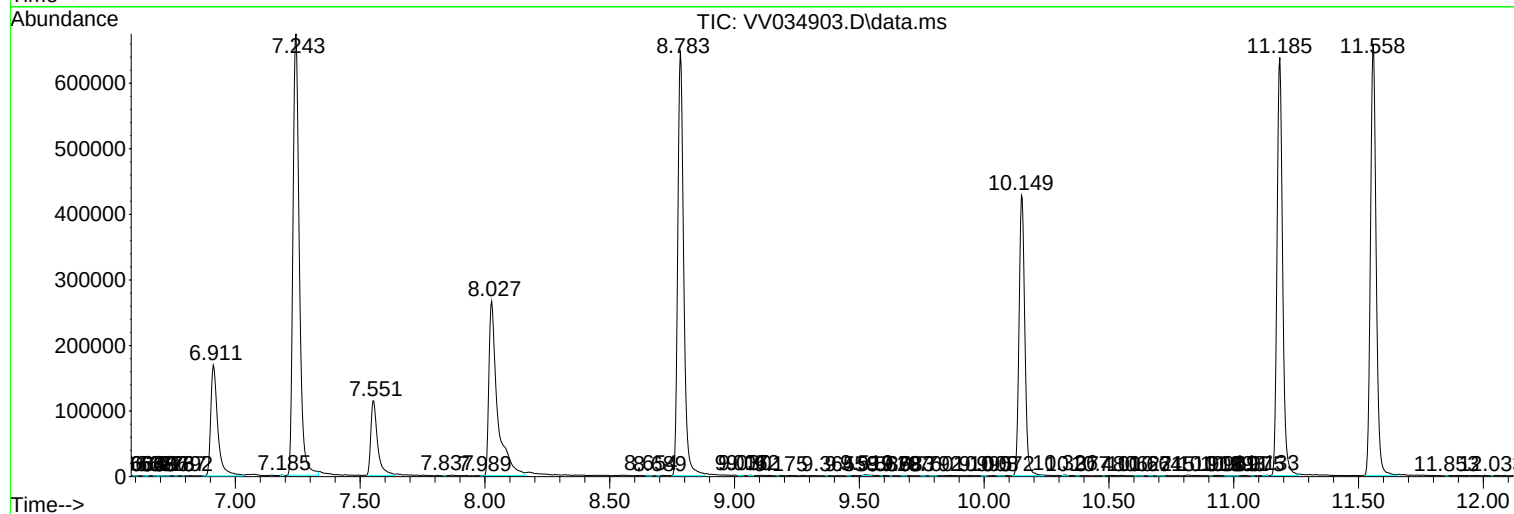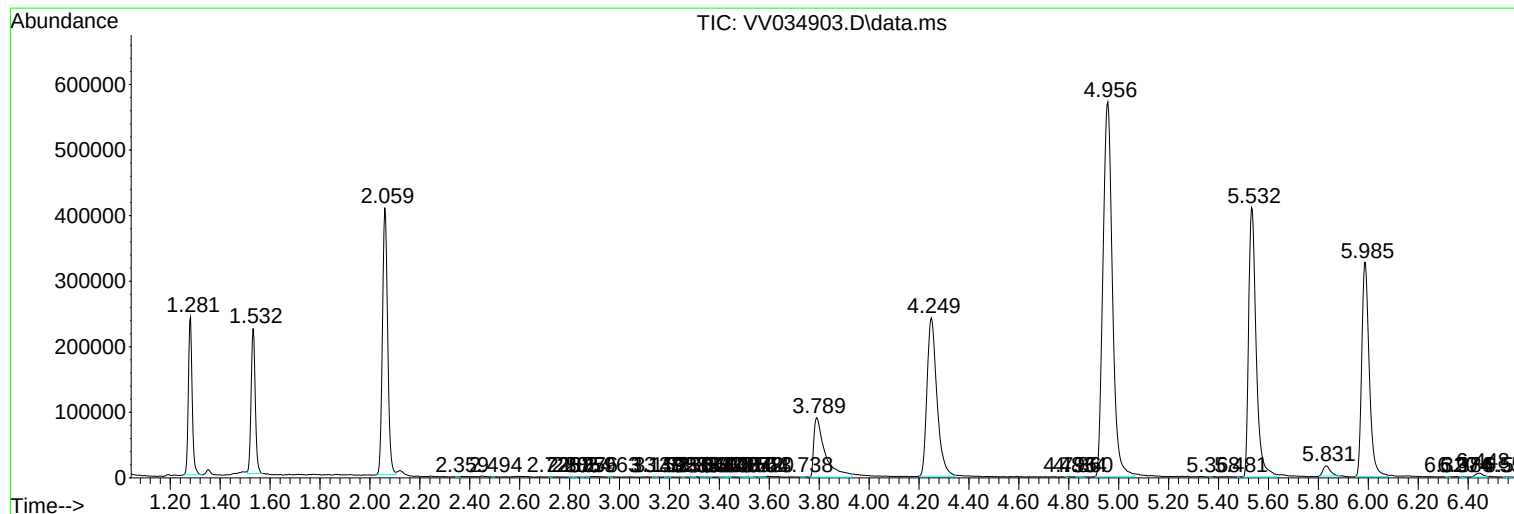

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034903.D
Acq On : 29 Mar 2024 12:20
Operator : SY/MD
Sample : P1886-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034903.D
Acq On : 29 Mar 2024 12:20
Operator : SY/MD
Sample : P1886-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------