

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034905.D
 Acq On : 29 Mar 2024 15:01
 Operator : SY/MD
 Sample : P1934-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	234540	240910	16.29%	2.380%
2	1.532	145	153	167	rVB	205593	242868	16.43%	2.399%
3	2.056	307	316	331	rBV	402785	591191	39.99%	5.840%
4	2.510	454	457	459	rBV2	507	264	0.02%	0.003%
5	2.568	473	475	480	rVB4	485	344	0.02%	0.003%
6	2.648	496	500	501	rBV2	178	132	0.01%	0.001%
7	2.725	522	524	525	rVB2	386	125	0.01%	0.001%
8	2.735	525	527	530	rBV	216	124	0.01%	0.001%
9	2.764	534	536	539	rVB2	468	207	0.01%	0.002%
10	2.812	549	551	552	rBV	308	149	0.01%	0.001%
11	2.905	578	580	582	rBV2	324	175	0.01%	0.002%
12	2.947	591	593	595	rBV	233	122	0.01%	0.001%
13	2.970	598	600	604	rBV3	389	300	0.02%	0.003%
14	3.040	618	622	623	rBV2	210	134	0.01%	0.001%
15	3.118	642	646	650	rBV2	543	476	0.03%	0.005%
16	3.150	654	656	661	rVV2	530	423	0.03%	0.004%
17	3.262	688	691	692	rBV	296	186	0.01%	0.002%
18	3.333	710	713	715	rBV2	276	196	0.01%	0.002%
19	3.346	715	717	724	rVV3	623	603	0.04%	0.006%
20	3.372	724	725	727	rVV3	374	150	0.01%	0.001%
21	3.400	730	734	735	rVV	314	248	0.02%	0.002%
22	3.494	760	763	764	rBV	318	155	0.01%	0.002%
23	3.542	776	778	784	rVB3	225	211	0.01%	0.002%
24	3.568	784	786	791	rBV2	310	292	0.02%	0.003%
25	3.609	796	799	803	rBV2	364	292	0.02%	0.003%
26	3.674	812	819	821	rBV3	561	618	0.04%	0.006%
27	3.783	844	853	889	rBV	92103	268200	18.14%	2.649%
28	4.243	982	996	1024	rBV	231104	595289	40.26%	5.881%
29	4.857	1185	1187	1190	rBV	260	154	0.01%	0.002%
30	4.950	1200	1216	1246	rBV2	560300	1478455	100.00%	14.605%
31	5.381	1347	1350	1354	rBV2	407	331	0.02%	0.003%
32	5.442	1365	1369	1370	rBV	516	363	0.02%	0.004%
33	5.490	1382	1384	1386	rVB	370	152	0.01%	0.002%
34	5.532	1386	1397	1435	rBV	245337	529424	35.81%	5.230%
35	5.825	1480	1488	1509	rBV3	13120	29744	2.01%	0.294%
36	5.982	1525	1537	1568	rBV	321443	668851	45.24%	6.607%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034905.D
 Acq On : 29 Mar 2024 15:01
 Operator : SY/MD
 Sample : P1934-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.404	1665	1668	1670	rBV3	523	299	0.02%	0.003%
38	6.429	1674	1676	1681	rVV2	513	284	0.02%	0.003%
39	6.471	1687	1689	1693	rVB2	516	302	0.02%	0.003%
40	6.526	1701	1706	1708	rBV3	285	199	0.01%	0.002%
41	6.542	1708	1711	1712	rBV	382	168	0.01%	0.002%
42	6.568	1717	1719	1723	rBV2	238	154	0.01%	0.002%
43	6.590	1723	1726	1729	rBV	400	266	0.02%	0.003%
44	6.613	1729	1733	1734	rBV2	366	263	0.02%	0.003%
45	6.625	1734	1737	1739	rVB3	493	329	0.02%	0.003%
46	6.641	1739	1742	1743	rBV	395	199	0.01%	0.002%
47	6.751	1773	1776	1778	rBV2	370	227	0.02%	0.002%
48	6.796	1788	1790	1791	rBV	576	206	0.01%	0.002%
49	6.912	1815	1826	1855	rBV	164065	322627	21.82%	3.187%
50	7.240	1916	1928	1959	rBV	658988	1169936	79.13%	11.557%
51	7.551	2015	2025	2052	rBV	115084	213319	14.43%	2.107%
52	7.969	2153	2155	2157	rBV	475	219	0.01%	0.002%
53	8.024	2163	2172	2212	rBV2	263996	615216	41.61%	6.077%
54	8.593	2347	2349	2353	rBV2	366	261	0.02%	0.003%
55	8.683	2375	2377	2379	rBV	264	142	0.01%	0.001%
56	8.696	2379	2381	2383	rBV	459	322	0.02%	0.003%
57	8.719	2386	2388	2390	rBV2	533	233	0.02%	0.002%
58	8.731	2390	2392	2394	rBV2	326	153	0.01%	0.002%
59	8.783	2397	2408	2433	rBV	391711	662043	44.78%	6.540%
60	9.034	2484	2486	2491	rVB3	471	338	0.02%	0.003%
61	9.059	2491	2494	2495	rBV	631	370	0.03%	0.004%
62	9.153	2520	2523	2526	rBV2	498	386	0.03%	0.004%
63	9.185	2529	2533	2536	rBV4	418	387	0.03%	0.004%
64	9.236	2544	2549	2551	rBV	550	384	0.03%	0.004%
65	9.281	2562	2563	2566	rVB3	419	214	0.01%	0.002%
66	9.333	2577	2579	2583	rVB	669	329	0.02%	0.003%
67	9.358	2584	2587	2590	rBV3	323	241	0.02%	0.002%
68	9.577	2653	2655	2657	rBV	387	177	0.01%	0.002%
69	9.616	2665	2667	2669	rBV2	672	212	0.01%	0.002%
70	9.645	2673	2676	2679	rVV	345	242	0.02%	0.002%
71	9.670	2682	2684	2689	rVV2	504	362	0.02%	0.004%
72	9.693	2689	2691	2694	rVB2	308	154	0.01%	0.002%
73	9.786	2718	2720	2722	rBV2	253	112	0.01%	0.001%
74	9.908	2756	2758	2760	rBV	311	182	0.01%	0.002%
75	9.934	2764	2766	2770	rVB2	431	240	0.02%	0.002%
76	9.960	2771	2774	2777	rBV3	336	199	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034905.D
 Acq On : 29 Mar 2024 15:01
 Operator : SY/MD
 Sample : P1934-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.069	2805	2808	2810	rBV	376	217	0.01%	0.002%
78	10.149	2822	2833	2848	rBV	427939	679387	45.95%	6.711%
79	10.551	2956	2958	2961	rVB	616	244	0.02%	0.002%
80	10.628	2979	2982	2986	rBV	304	269	0.02%	0.003%
81	10.780	3024	3029	3031	rBV2	529	384	0.03%	0.004%
82	10.812	3036	3039	3040	rBV	289	140	0.01%	0.001%
83	10.857	3045	3053	3062	rBV2	4791	7619	0.52%	0.075%
84	10.921	3071	3073	3074	rBV2	286	134	0.01%	0.001%
85	10.931	3074	3076	3079	rVB2	467	270	0.02%	0.003%
86	10.963	3084	3086	3088	rBV	267	141	0.01%	0.001%
87	11.034	3105	3108	3112	rBV2	301	278	0.02%	0.003%
88	11.095	3125	3127	3132	rBV3	398	360	0.02%	0.004%
89	11.136	3136	3140	3143	rVB4	681	487	0.03%	0.005%
90	11.185	3144	3155	3179	rBV	395355	630993	42.68%	6.233%
91	11.426	3228	3230	3231	rBV	324	149	0.01%	0.001%
92	11.558	3260	3271	3298	rBV	637378	1017617	68.83%	10.053%
93	12.008	3408	3411	3412	rBV	422	170	0.01%	0.002%
94	12.117	3442	3445	3448	rBV2	539	396	0.03%	0.004%
95	12.532	3571	3574	3577	rBV	410	256	0.02%	0.003%
96	12.792	3650	3655	3664	rBV3	422	602	0.04%	0.006%
97	13.204	3773	3783	3797	rBV	38229	61634	4.17%	0.609%
98	13.442	3848	3857	3871	rBV	45023	76360	5.16%	0.754%
99	13.596	3902	3905	3909	rBV	609	468	0.03%	0.005%
100	15.140	4381	4385	4386	rBV	722	550	0.04%	0.005%




Sum of corrected areas: 10122879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034905.D
Acq On : 29 Mar 2024 15:01
Operator : SY/MD
Sample : P1934-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

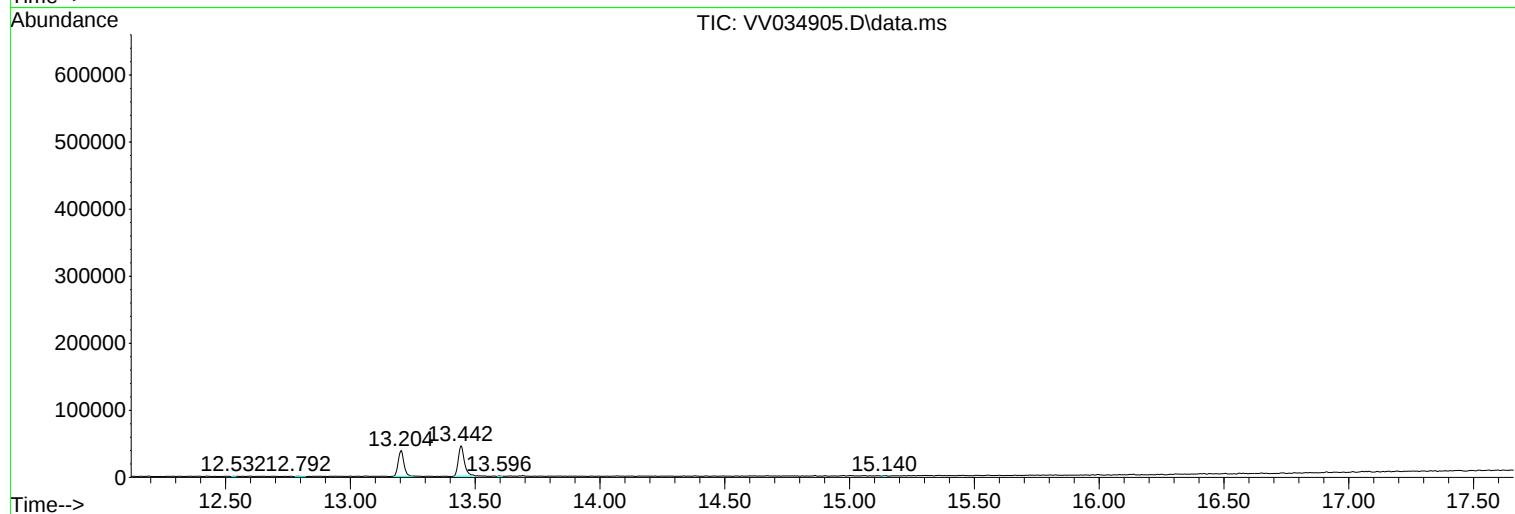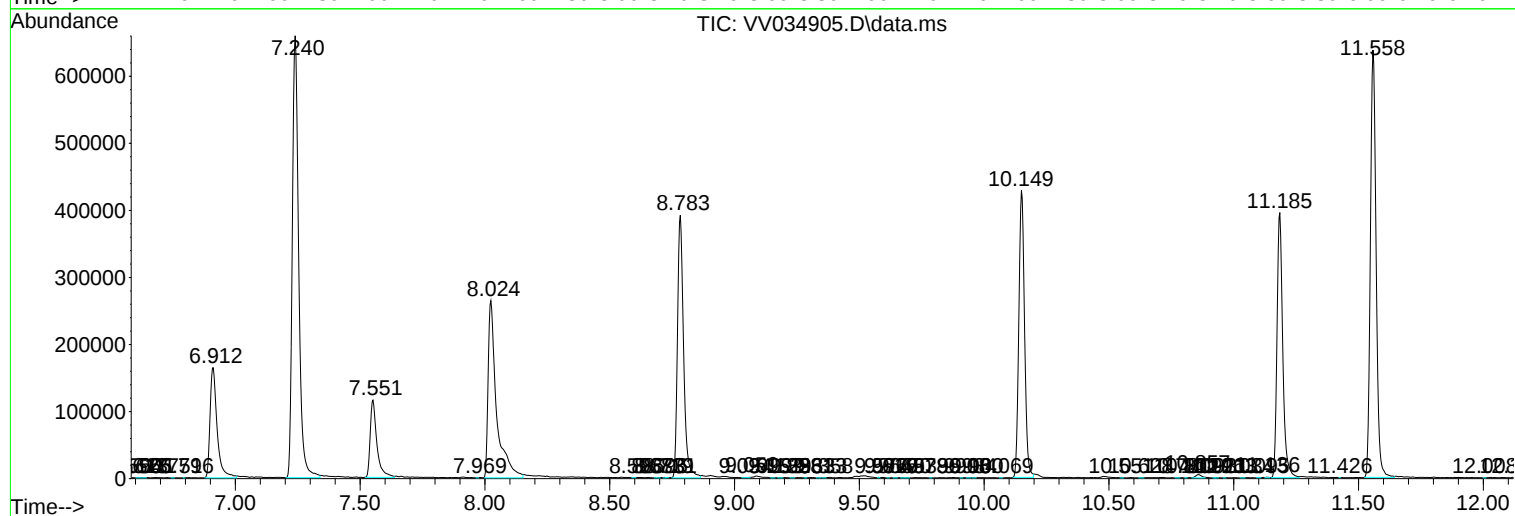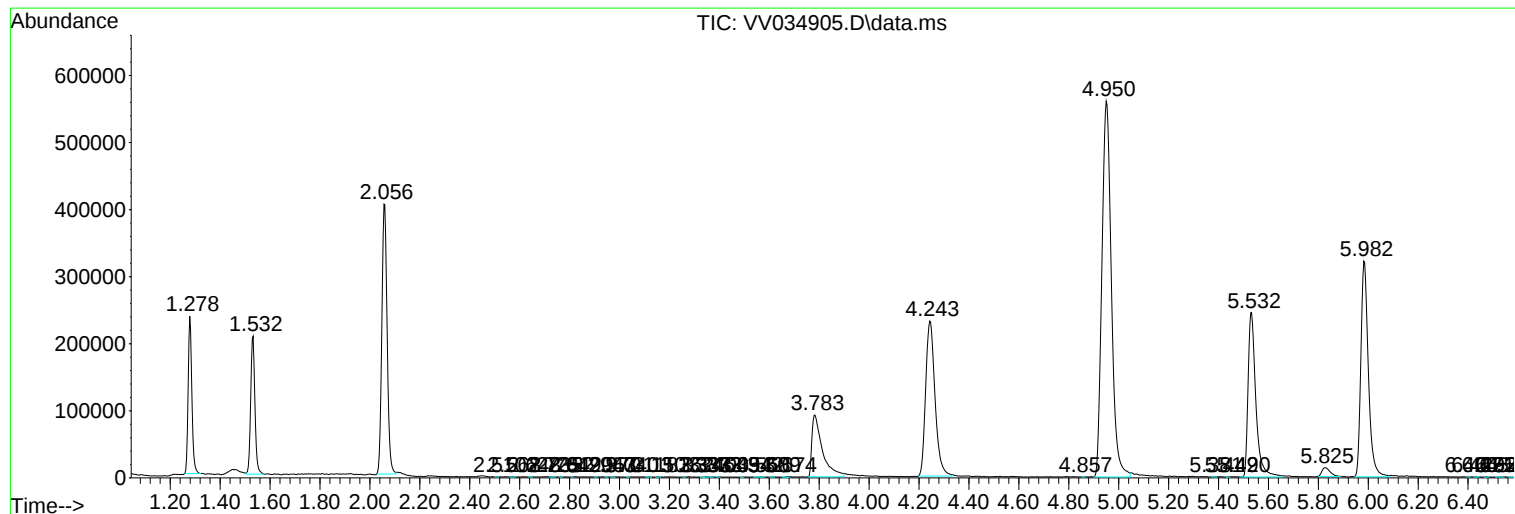

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034905.D
Acq On : 29 Mar 2024 15:01
Operator : SY/MD
Sample : P1934-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034905.D
Acq On : 29 Mar 2024 15:01
Operator : SY/MD
Sample : P1934-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc