

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034906.D
 Acq On : 29 Mar 2024 15:25
 Operator : SY/MD
 Sample : P1934-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	224650	237053	4.02%	1.295%
2	1.532	145	153	167	rVB	197202	229758	3.90%	1.256%
3	2.060	307	317	328	rBV	388619	564731	9.58%	3.086%
4	2.519	455	460	462	rBV2	548	457	0.01%	0.002%
5	2.706	511	518	520	rBV4	586	569	0.01%	0.003%
6	2.770	535	538	539	rBV	282	154	0.00%	0.001%
7	2.835	555	558	560	rBV2	282	182	0.00%	0.001%
8	2.867	565	568	572	rBV2	429	343	0.01%	0.002%
9	2.915	581	583	586	rBV2	278	135	0.00%	0.001%
10	3.005	605	611	616	rVB2	326	382	0.01%	0.002%
11	3.028	616	618	622	rBV3	485	415	0.01%	0.002%
12	3.089	634	637	640	rBV2	188	130	0.00%	0.001%
13	3.101	640	641	644	rVB	190	96	0.00%	0.001%
14	3.127	647	649	652	rBV	171	132	0.00%	0.001%
15	3.159	656	659	660	rBV	297	177	0.00%	0.001%
16	3.179	662	665	669	rVB2	395	300	0.01%	0.002%
17	3.262	686	691	692	rBV	468	362	0.01%	0.002%
18	3.349	715	718	720	rBV	273	170	0.00%	0.001%
19	3.368	721	724	726	rBV	330	229	0.00%	0.001%
20	3.478	756	758	761	rBV2	154	109	0.00%	0.001%
21	3.494	761	763	766	rBV	409	234	0.00%	0.001%
22	3.571	784	787	792	rBV3	282	198	0.00%	0.001%
23	3.635	805	807	809	rVB2	299	133	0.00%	0.001%
24	3.687	820	823	825	rBV2	349	215	0.00%	0.001%
25	3.735	835	838	842	rBV2	434	325	0.01%	0.002%
26	3.786	842	854	898	rBV2	115313	367249	6.23%	2.007%
27	4.246	983	997	1023	rBV	224690	569285	9.66%	3.111%
28	4.687	1132	1134	1137	rBV3	444	255	0.00%	0.001%
29	4.796	1166	1168	1172	rVB3	452	183	0.00%	0.001%
30	4.828	1172	1178	1180	rBV	475	509	0.01%	0.003%
31	4.953	1200	1217	1268	rBV2	550375	1507868	25.59%	8.240%
32	5.381	1347	1350	1354	rVB3	540	377	0.01%	0.002%
33	5.532	1386	1397	1428	rBV	408571	843681	14.32%	4.611%
34	5.831	1480	1490	1505	rBV2	12541	27353	0.46%	0.149%
35	5.986	1524	1538	1565	rBV	313568	657879	11.16%	3.595%
36	6.301	1634	1636	1639	rVB3	414	215	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034906.D
 Acq On : 29 Mar 2024 15:25
 Operator : SY/MD
 Sample : P1934-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.323	1639	1643	1645	rBV2	573	310	0.01%	0.002%
38	6.359	1650	1654	1655	rBV	443	282	0.00%	0.002%
39	6.458	1679	1685	1687	rBV3	659	600	0.01%	0.003%
40	6.545	1708	1712	1714	rBV3	389	315	0.01%	0.002%
41	6.619	1731	1735	1739	rBV4	624	428	0.01%	0.002%
42	6.642	1739	1742	1744	rBV2	418	322	0.01%	0.002%
43	6.683	1754	1755	1759	rVB3	474	276	0.00%	0.002%
44	6.744	1770	1774	1780	rBV6	652	776	0.01%	0.004%
45	6.799	1786	1791	1793	rBV3	406	299	0.01%	0.002%
46	6.841	1802	1804	1806	rBV	197	113	0.00%	0.001%
47	6.863	1809	1811	1813	rVB	320	121	0.00%	0.001%
48	6.876	1813	1815	1816	rBV	234	100	0.00%	0.001%
49	6.912	1816	1826	1859	rBV	161354	313220	5.31%	1.712%
50	7.108	1884	1887	1890	rBV4	798	543	0.01%	0.003%
51	7.243	1918	1929	1957	rBV	637866	1130782	19.19%	6.180%
52	7.551	2016	2025	2044	rBV	110799	199717	3.39%	1.091%
53	7.873	2122	2125	2127	rBV2	618	325	0.01%	0.002%
54	8.024	2162	2172	2215	rBV2	293264	636571	10.80%	3.479%
55	8.535	2329	2331	2333	rBV3	492	213	0.00%	0.001%
56	8.645	2363	2365	2368	rBV2	515	321	0.01%	0.002%
57	8.783	2397	2408	2412	rBV	680294	1016292	17.25%	5.554%
58	9.182	2530	2532	2535	rBV3	483	262	0.00%	0.001%
59	9.375	2589	2592	2594	rBV	349	173	0.00%	0.001%
60	9.391	2594	2597	2598	rBV	295	141	0.00%	0.001%
61	9.439	2608	2612	2613	rBV2	448	299	0.01%	0.002%
62	9.474	2621	2623	2624	rBV2	394	139	0.00%	0.001%
63	9.612	2663	2666	2668	rBV2	571	393	0.01%	0.002%
64	9.699	2691	2693	2694	rBV	433	184	0.00%	0.001%
65	9.738	2702	2705	2707	rBV2	402	223	0.00%	0.001%
66	9.831	2731	2734	2735	rBV	324	145	0.00%	0.001%
67	9.863	2743	2744	2746	rBV2	272	135	0.00%	0.001%
68	9.956	2770	2773	2776	rBV2	381	319	0.01%	0.002%
69	9.995	2782	2785	2787	rBV	243	174	0.00%	0.001%
70	10.149	2822	2833	2860	rBV	427993	683962	11.61%	3.738%
71	10.394	2907	2909	2911	rBV	400	155	0.00%	0.001%
72	10.419	2916	2917	2924	rVB2	474	330	0.01%	0.002%
73	10.477	2933	2935	2937	rBV	486	239	0.00%	0.001%
74	10.612	2975	2977	2979	rBV	425	138	0.00%	0.001%
75	10.664	2991	2993	2995	rBV2	290	127	0.00%	0.001%
76	10.693	3000	3002	3004	rVB2	359	135	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034906.D
 Acq On : 29 Mar 2024 15:25
 Operator : SY/MD
 Sample : P1934-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.715	3006	3009	3011	rBV	318	190	0.00%	0.001%
78	10.799	3032	3035	3039	rBV2	515	456	0.01%	0.002%
79	10.850	3048	3051	3052	rBV2	832	418	0.01%	0.002%
80	11.005	3096	3099	3101	rVB	342	167	0.00%	0.001%
81	11.021	3101	3104	3107	rVB2	399	252	0.00%	0.001%
82	11.117	3123	3134	3145	rBV	123001	195413	3.32%	1.068%
83	11.185	3145	3155	3157	rBV	753655	914666	15.52%	4.998%
84	11.574	3260	3276	3314	rBV2	3270902	5893164	100.00%	32.205%
85	11.905	3377	3379	3381	rBV2	474	266	0.00%	0.001%
86	12.005	3408	3410	3411	rBV	469	161	0.00%	0.001%
87	12.149	3454	3455	3457	rBV	295	139	0.00%	0.001%
88	12.345	3510	3516	3530	rVB9	3205	5320	0.09%	0.029%
89	12.458	3549	3551	3552	rBV	351	142	0.00%	0.001%
90	12.506	3564	3566	3569	rBV2	400	356	0.01%	0.002%
91	12.577	3579	3588	3608	rBV2	38237	72607	1.23%	0.397%
92	12.972	3708	3711	3714	rBV3	481	290	0.00%	0.002%
93	13.198	3769	3781	3811	rBV	925457	1426792	24.21%	7.797%
94	13.445	3850	3858	3872	rVB2	19332	33488	0.57%	0.183%
95	13.628	3910	3915	3917	rBV2	795	608	0.01%	0.003%
96	13.677	3917	3930	3956	rVV	398211	633116	10.74%	3.460%
97	14.050	4044	4046	4047	rBV2	669	328	0.01%	0.002%
98	14.095	4052	4060	4073	rBV4	8595	16953	0.29%	0.093%
99	14.760	4261	4267	4277	rVB4	13188	20118	0.34%	0.110%
100	15.336	4436	4446	4459	rBV2	50693	81964	1.39%	0.448%

Sum of corrected areas: 18298816




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034906.D
Acq On : 29 Mar 2024 15:25
Operator : SY/MD
Sample : P1934-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

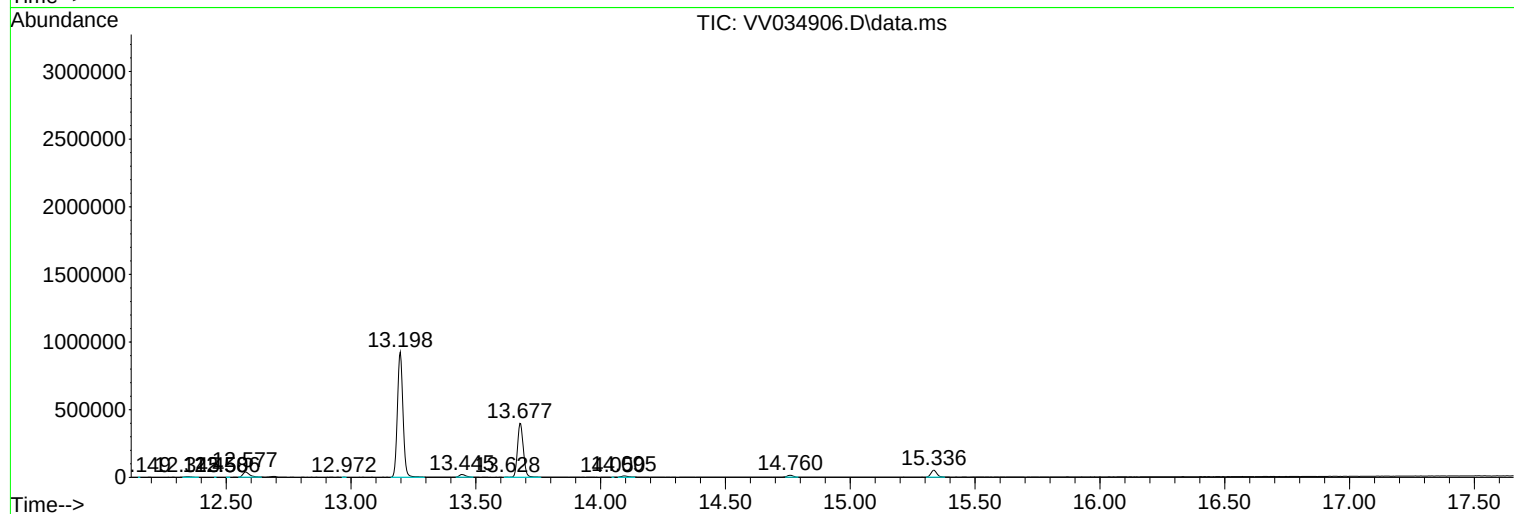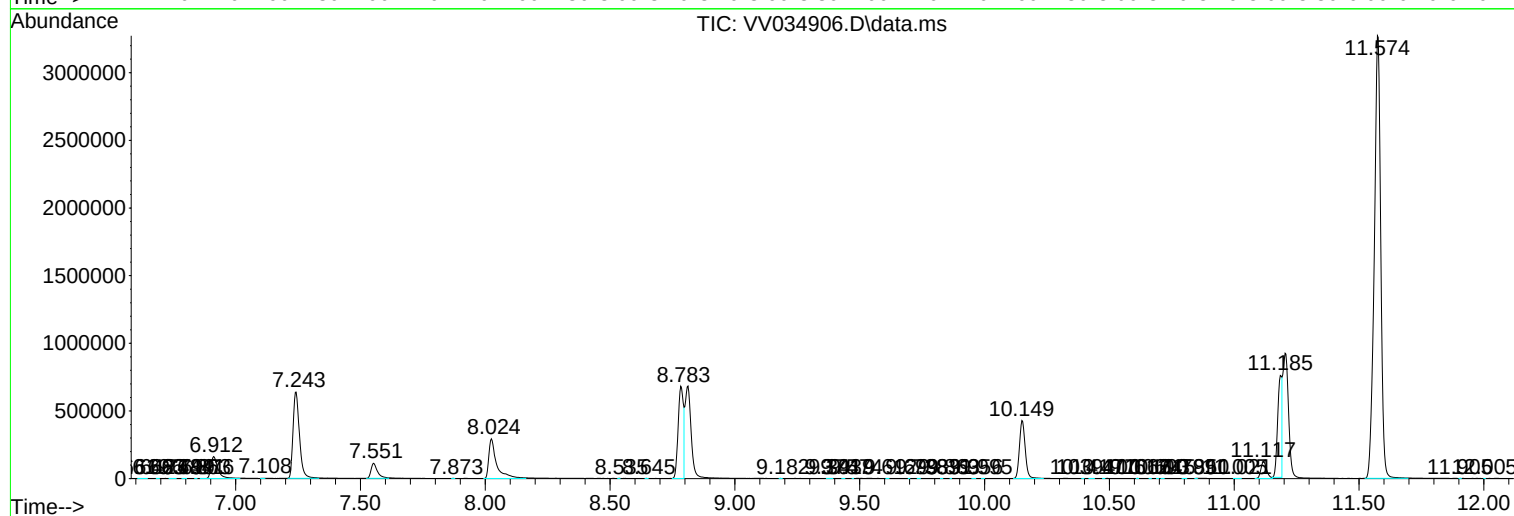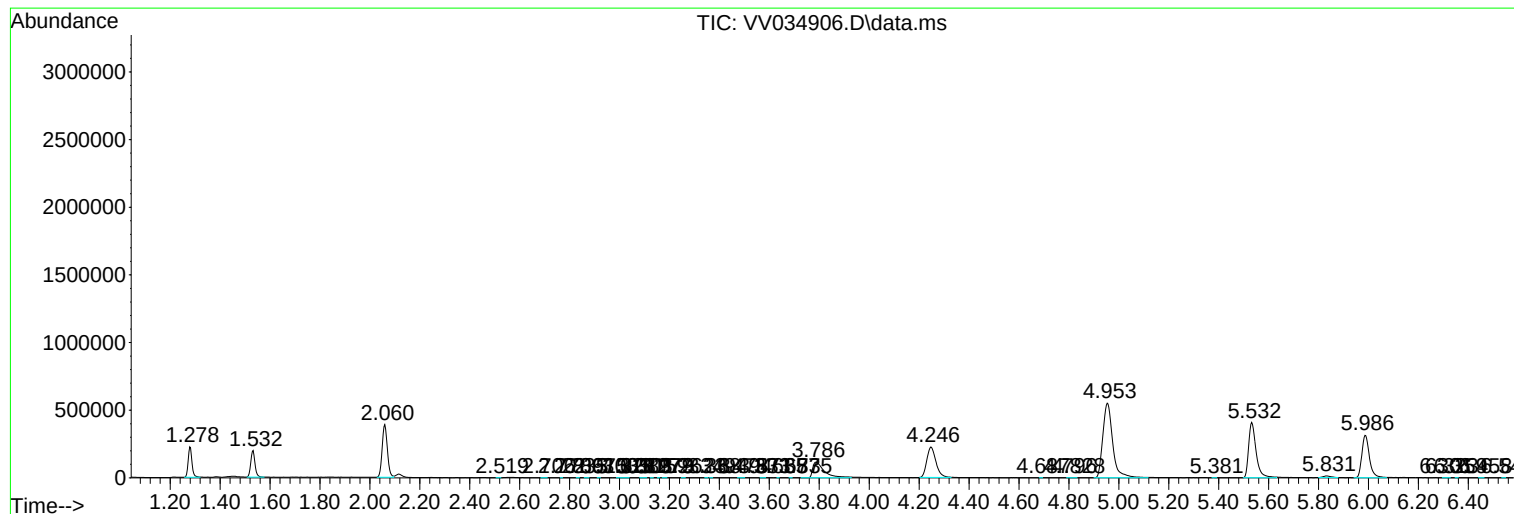

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034906.D
Acq On : 29 Mar 2024 15:25
Operator : SY/MD
Sample : P1934-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034906.D
Acq On : 29 Mar 2024 15:25
Operator : SY/MD
Sample : P1934-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------