

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034908.D
 Acq On : 29 Mar 2024 16:13
 Operator : SY/MD
 Sample : P1934-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	214353	224362	16.36%	2.226%
2	1.532	146	153	171	rVB	183525	220827	16.10%	2.191%
3	2.059	308	317	334	rBV	366096	524813	38.26%	5.206%
4	2.555	463	471	473	rBV6	2123	2517	0.18%	0.025%
5	2.613	487	489	490	rBV2	424	215	0.02%	0.002%
6	2.706	514	518	520	rBV	413	301	0.02%	0.003%
7	2.789	541	544	546	rBV2	387	273	0.02%	0.003%
8	2.802	546	548	550	rVV2	552	264	0.02%	0.003%
9	2.870	566	569	572	rBV	417	311	0.02%	0.003%
10	2.895	575	577	580	rBV	355	249	0.02%	0.002%
11	3.011	609	613	614	rBV	279	186	0.01%	0.002%
12	3.069	629	631	636	rVB2	562	226	0.02%	0.002%
13	3.104	639	642	643	rBV	320	218	0.02%	0.002%
14	3.220	676	678	683	rVB	472	281	0.02%	0.003%
15	3.249	683	687	688	rBV2	226	173	0.01%	0.002%
16	3.294	698	701	703	rBV2	352	190	0.01%	0.002%
17	3.330	709	712	714	rBV2	265	180	0.01%	0.002%
18	3.365	721	723	725	rBV2	503	269	0.02%	0.003%
19	3.471	755	756	761	rVB2	350	245	0.02%	0.002%
20	3.497	761	764	767	rBV2	246	186	0.01%	0.002%
21	3.686	820	823	829	rVB2	328	276	0.02%	0.003%
22	3.722	829	834	835	rBV2	658	470	0.03%	0.005%
23	3.793	846	856	902	rBV2	110591	359184	26.18%	3.563%
24	4.249	981	998	1035	rBV	214147	560079	40.83%	5.556%
25	4.793	1165	1167	1170	rBV2	281	169	0.01%	0.002%
26	4.889	1194	1197	1199	rBV2	314	205	0.01%	0.002%
27	4.956	1199	1218	1250	rBV2	526072	1371817	100.00%	13.609%
28	5.429	1363	1365	1369	rBV2	619	435	0.03%	0.004%
29	5.535	1386	1398	1430	rBV	329303	698425	50.91%	6.929%
30	5.831	1481	1490	1511	rBV	13722	31384	2.29%	0.311%
31	5.931	1518	1521	1524	rVB2	700	385	0.03%	0.004%
32	5.989	1524	1539	1566	rBV	297483	626951	45.70%	6.220%
33	6.313	1638	1640	1642	rVB	453	167	0.01%	0.002%
34	6.346	1647	1650	1652	rVB2	498	241	0.02%	0.002%
35	6.365	1652	1656	1660	rBV3	583	424	0.03%	0.004%
36	6.413	1667	1671	1674	rBV3	490	360	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034908.D
 Acq On : 29 Mar 2024 16:13
 Operator : SY/MD
 Sample : P1934-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.448	1678	1682	1688	rBV3	363	354	0.03%	0.004%
38	6.503	1697	1699	1702	rVB3	498	247	0.02%	0.002%
39	6.667	1747	1750	1753	rBV3	461	376	0.03%	0.004%
40	6.744	1769	1774	1778	rBV5	669	600	0.04%	0.006%
41	6.834	1799	1802	1805	rBV	349	210	0.02%	0.002%
42	6.911	1815	1826	1858	rBV	148602	293827	21.42%	2.915%
43	7.243	1918	1929	1950	rBV	600175	1057389	77.08%	10.490%
44	7.554	2016	2026	2053	rBV2	103079	193882	14.13%	1.923%
45	7.866	2119	2123	2124	rBV2	530	351	0.03%	0.003%
46	7.911	2134	2137	2138	rBV	436	218	0.02%	0.002%
47	8.027	2163	2173	2210	rBV2	262699	591150	43.09%	5.865%
48	8.432	2297	2299	2301	rVB2	795	335	0.02%	0.003%
49	8.693	2375	2380	2383	rBV4	559	406	0.03%	0.004%
50	8.783	2397	2408	2438	rBV	522016	874784	63.77%	8.678%
51	9.021	2479	2482	2485	rBV3	881	680	0.05%	0.007%
52	9.091	2501	2504	2509	rBV3	660	644	0.05%	0.006%
53	9.136	2516	2518	2521	rBV2	468	272	0.02%	0.003%
54	9.197	2534	2537	2543	rBV2	556	597	0.04%	0.006%
55	9.271	2556	2560	2566	rBV2	748	616	0.04%	0.006%
56	9.300	2566	2569	2572	rBV3	398	246	0.02%	0.002%
57	9.336	2577	2580	2582	rVB	289	193	0.01%	0.002%
58	9.390	2593	2597	2601	rBV2	568	428	0.03%	0.004%
59	9.419	2601	2606	2609	rVB2	610	506	0.04%	0.005%
60	9.468	2619	2621	2626	rVB3	475	389	0.03%	0.004%
61	9.493	2627	2629	2631	rBV2	417	239	0.02%	0.002%
62	9.535	2639	2642	2644	rBV2	378	190	0.01%	0.002%
63	9.561	2644	2650	2652	rBV2	254	219	0.02%	0.002%
64	9.599	2660	2662	2667	rBV	350	272	0.02%	0.003%
65	9.657	2678	2680	2686	rBV	215	170	0.01%	0.002%
66	9.705	2693	2695	2698	rVB	423	184	0.01%	0.002%
67	9.722	2698	2700	2702	rBV2	298	180	0.01%	0.002%
68	9.834	2730	2735	2736	rBV	484	310	0.02%	0.003%
69	9.863	2741	2744	2746	rBV	255	180	0.01%	0.002%
70	9.882	2746	2750	2753	rVB3	542	456	0.03%	0.005%
71	9.905	2753	2757	2760	rBV2	304	186	0.01%	0.002%
72	9.921	2760	2762	2763	rBV2	418	192	0.01%	0.002%
73	10.033	2794	2797	2801	rVB2	624	465	0.03%	0.005%
74	10.152	2820	2834	2855	rBV	402014	635485	46.32%	6.304%
75	10.355	2894	2897	2898	rBV2	482	245	0.02%	0.002%
76	10.461	2926	2930	2932	rBV	382	310	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034908.D
 Acq On : 29 Mar 2024 16:13
 Operator : SY/MD
 Sample : P1934-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.500	2937	2942	2945	rBV4	598	568	0.04%	0.006%
78	10.567	2961	2963	2966	rVB3	343	188	0.01%	0.002%
79	10.596	2969	2972	2973	rBV	372	186	0.01%	0.002%
80	10.805	3031	3037	3042	rBV3	414	489	0.04%	0.005%
81	10.847	3048	3050	3053	rBV	284	192	0.01%	0.002%
82	10.914	3069	3071	3075	rBV	394	246	0.02%	0.002%
83	10.966	3085	3087	3090	rBV2	562	235	0.02%	0.002%
84	11.120	3132	3135	3138	rBV2	774	469	0.03%	0.005%
85	11.185	3144	3155	3180	rBV	522206	821378	59.88%	8.149%
86	11.558	3260	3271	3291	rBV	582540	936443	68.26%	9.290%
87	11.738	3324	3327	3329	rBV2	847	485	0.04%	0.005%
88	12.156	3453	3457	3461	rBV3	368	336	0.02%	0.003%
89	12.271	3490	3493	3495	rBV	425	297	0.02%	0.003%
90	12.361	3517	3521	3523	rBV	447	352	0.03%	0.003%
91	12.432	3540	3543	3545	rBV2	414	329	0.02%	0.003%
92	12.500	3562	3564	3567	rBV	362	210	0.02%	0.002%
93	12.586	3589	3591	3592	rBV	395	179	0.01%	0.002%
94	12.911	3689	3692	3695	rBV2	629	467	0.03%	0.005%
95	12.979	3708	3713	3714	rBV	563	459	0.03%	0.005%
96	13.130	3758	3760	3763	rVB2	474	241	0.02%	0.002%
97	13.207	3775	3784	3793	rBV4	11361	19013	1.39%	0.189%
98	13.455	3852	3861	3870	rBV2	3191	5031	0.37%	0.050%
99	13.622	3908	3913	3914	rBV2	697	542	0.04%	0.005%
100	13.686	3928	3933	3943	rVB8	4329	6475	0.47%	0.064%




Sum of corrected areas: 10080051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034908.D
Acq On : 29 Mar 2024 16:13
Operator : SY/MD
Sample : P1934-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

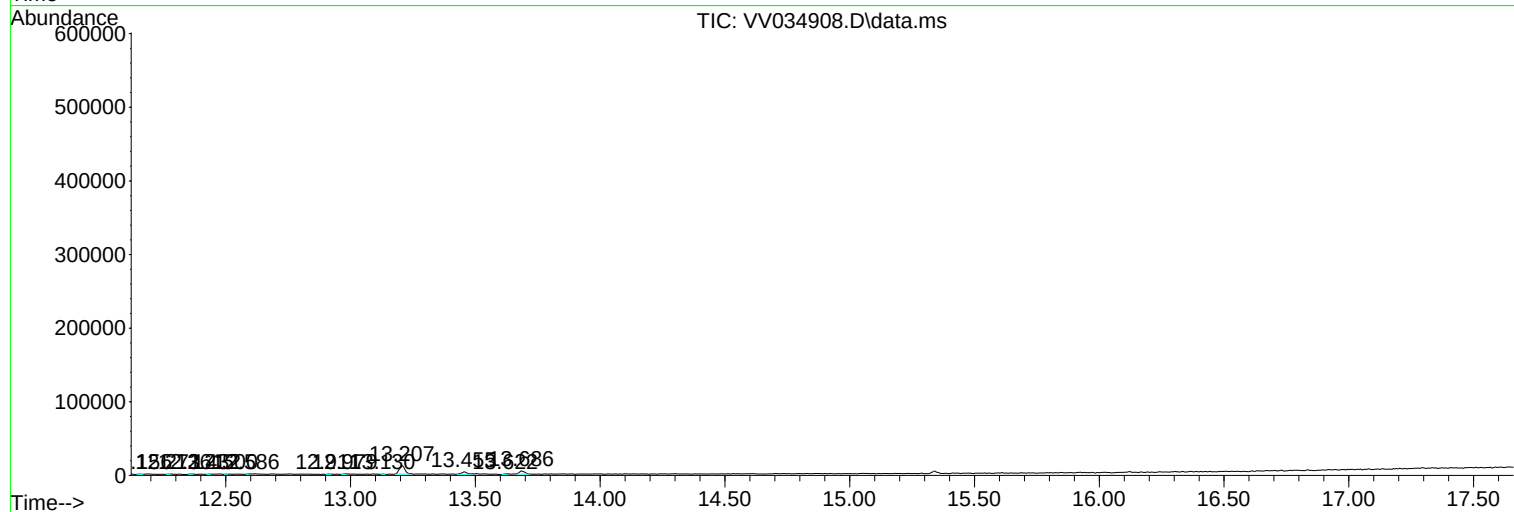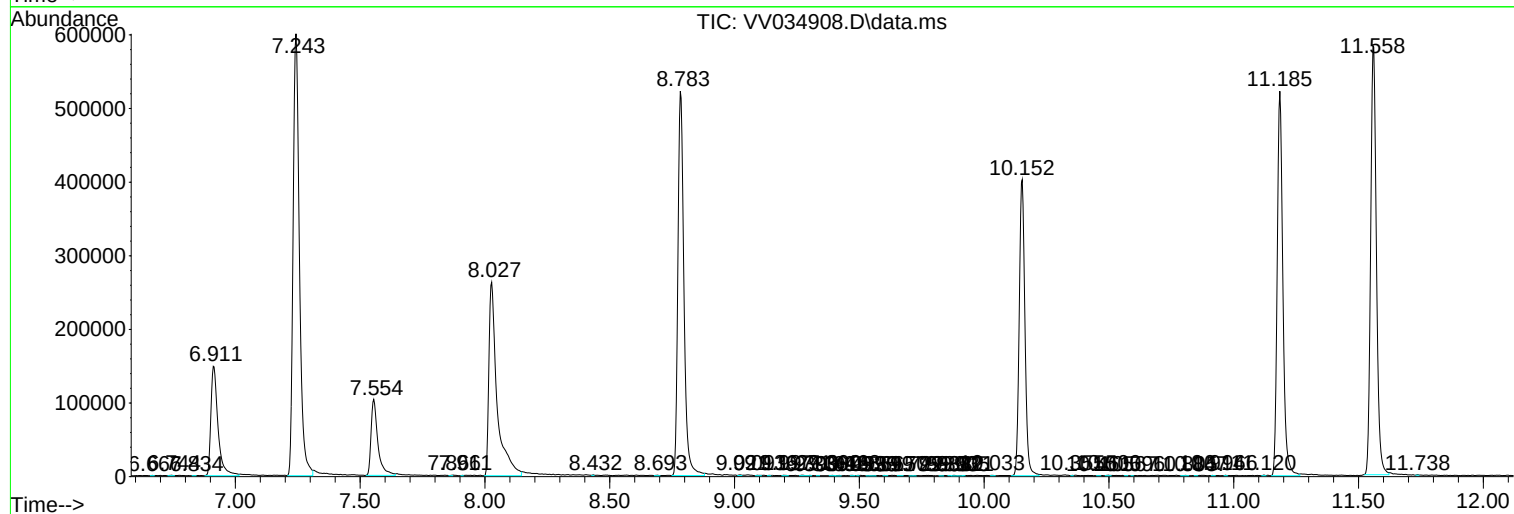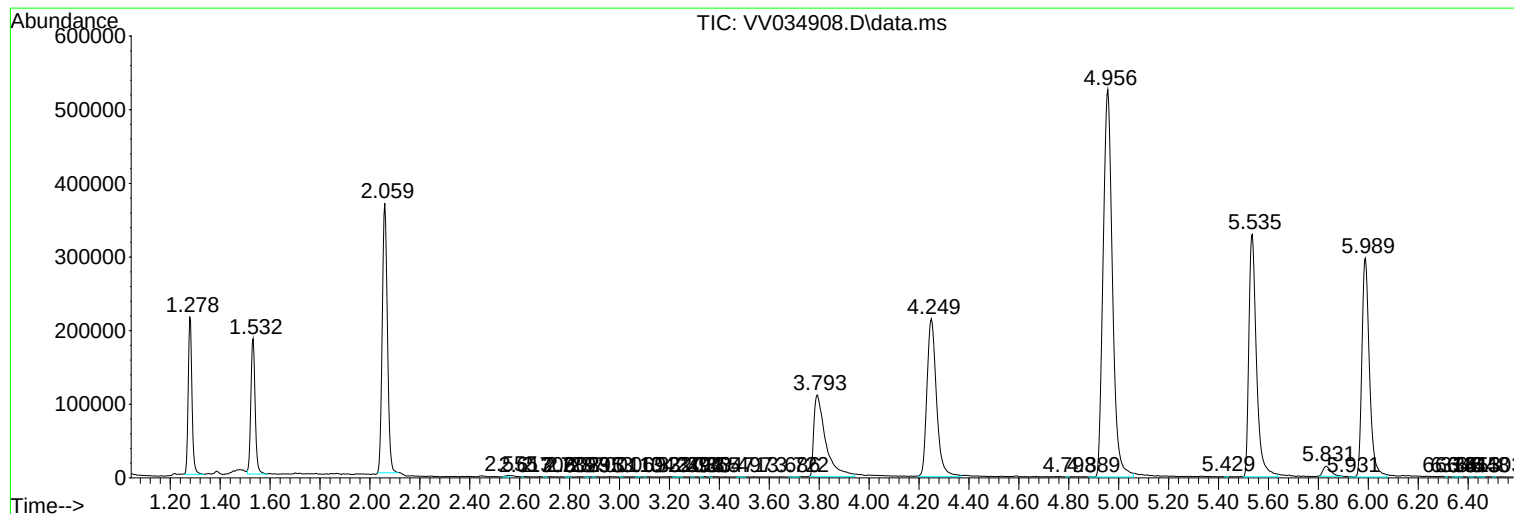

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034908.D
Acq On : 29 Mar 2024 16:13
Operator : SY/MD
Sample : P1934-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034908.D
Acq On : 29 Mar 2024 16:13
Operator : SY/MD
Sample : P1934-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
